
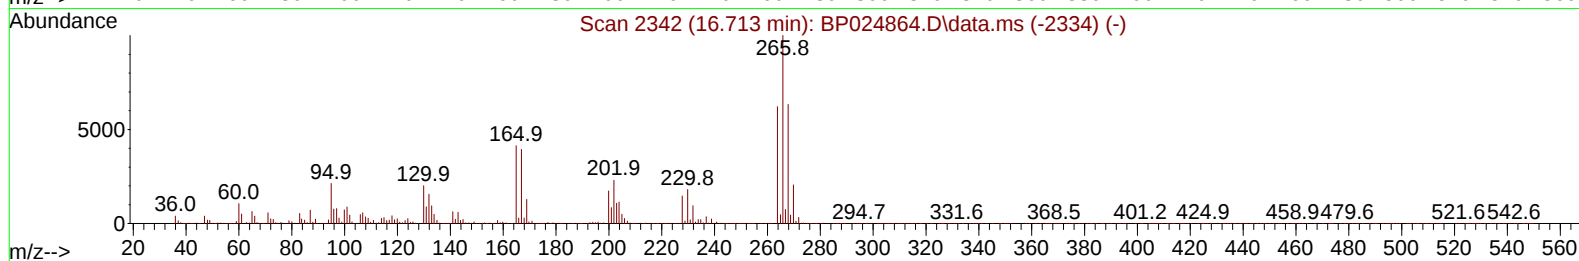
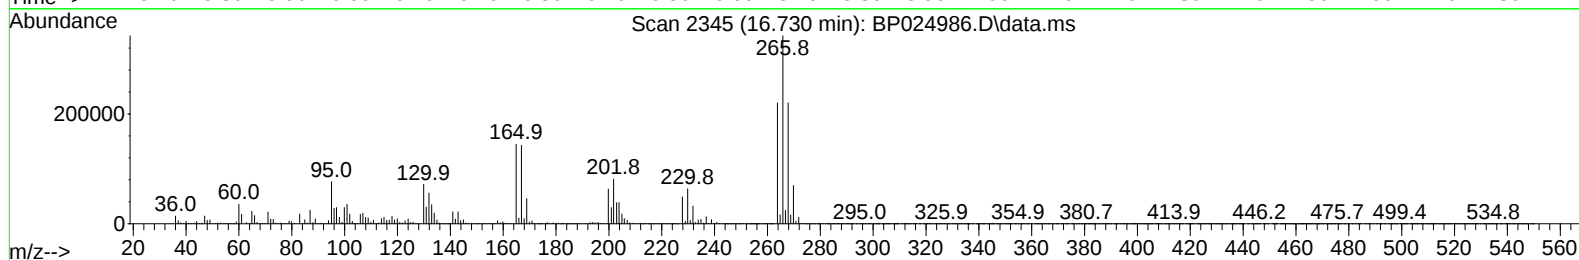


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061825\
Data File : BP024986.D
Acq On : 18 Jun 2025 09:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 11:34:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

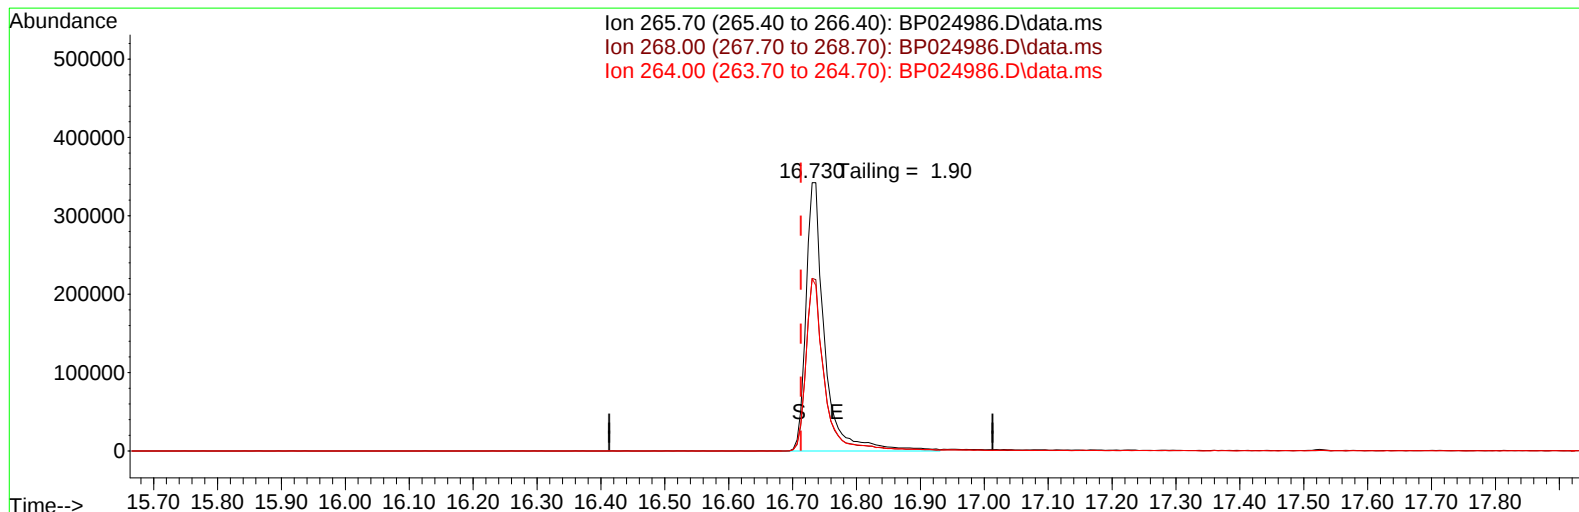

TIC: BP024986.D\data.ms

(70) Pentachlorophenol (C)




16.730min (+ 0.017) 2136417.31 ng

response 695724

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.34
264.00	62.10	64.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061825\
Data File : BP024986.D
Acq On : 18 Jun 2025 09:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 11:34:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

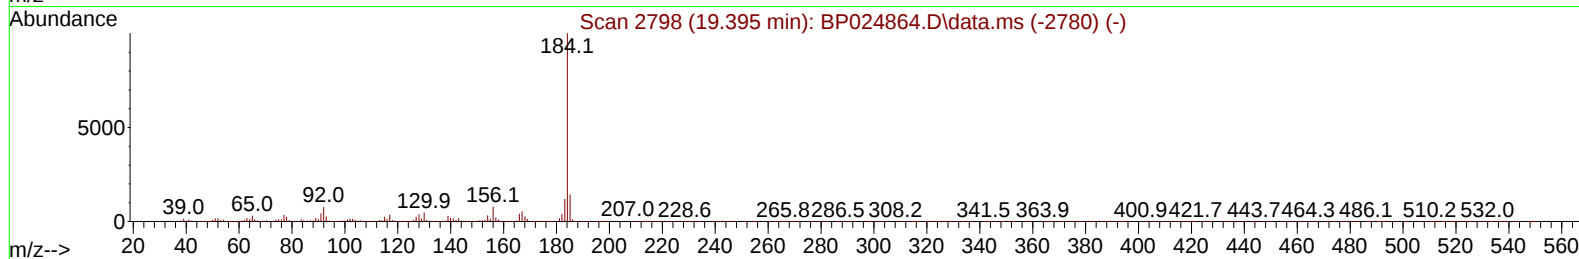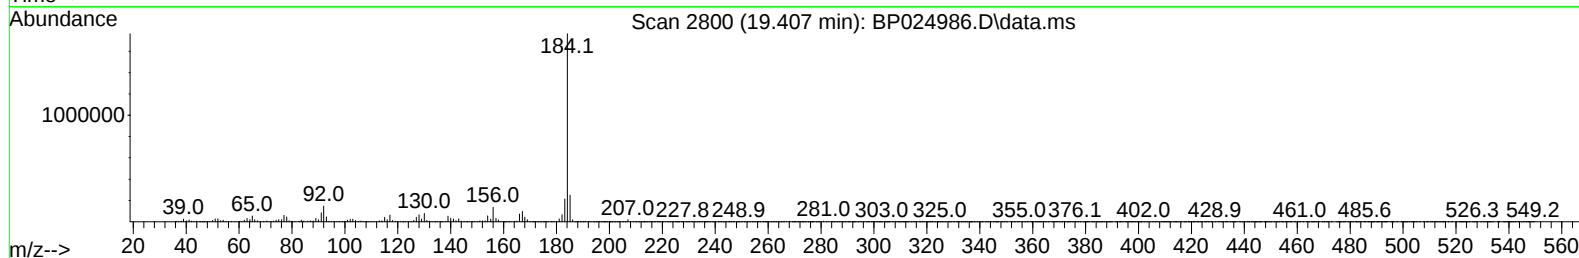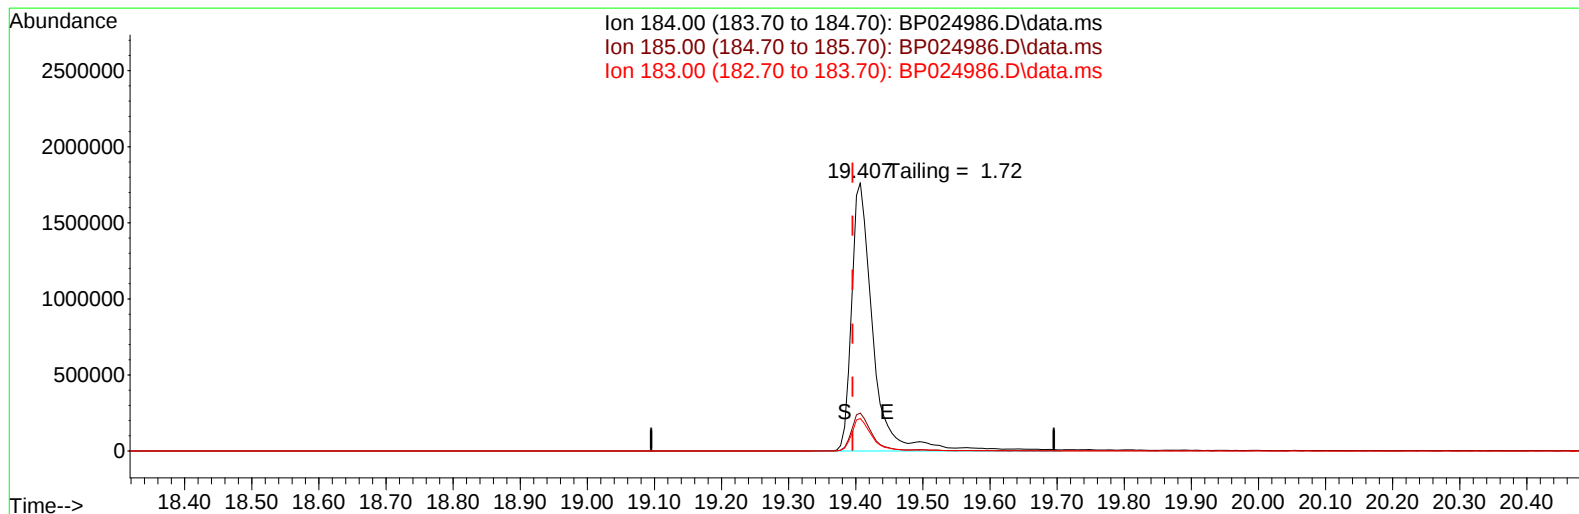

TIC: BP024986.D\data.ms

(77) Benzidine**19.407min (+ 0.012) 430098.83 ng****response 3649895**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.16
183.00	11.90	12.09
0.00	0.00	0.00