
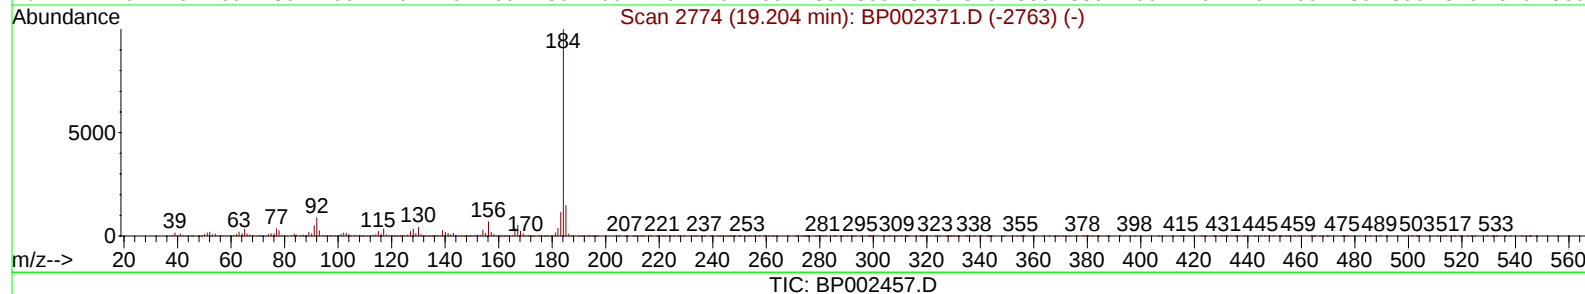
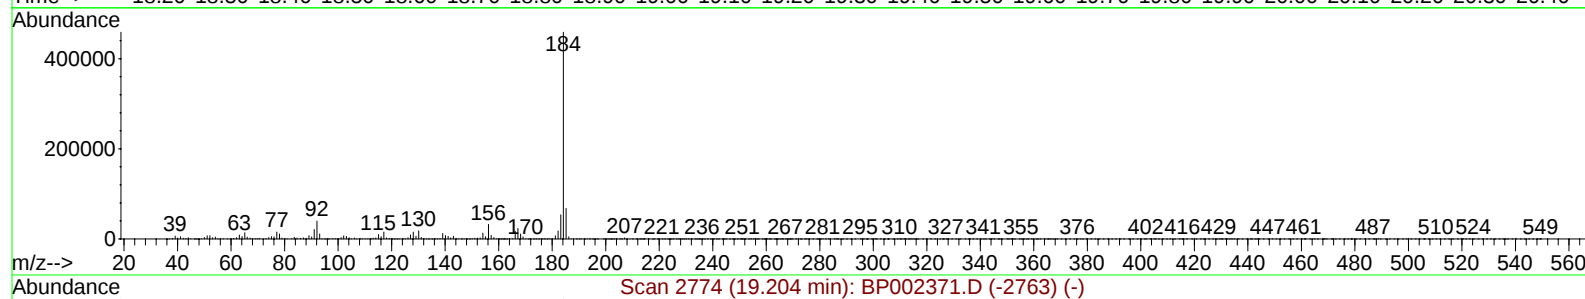


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061920\
 Data File : BP002457.D
 Acq On : 19 Jun 2020 14:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 19:15:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

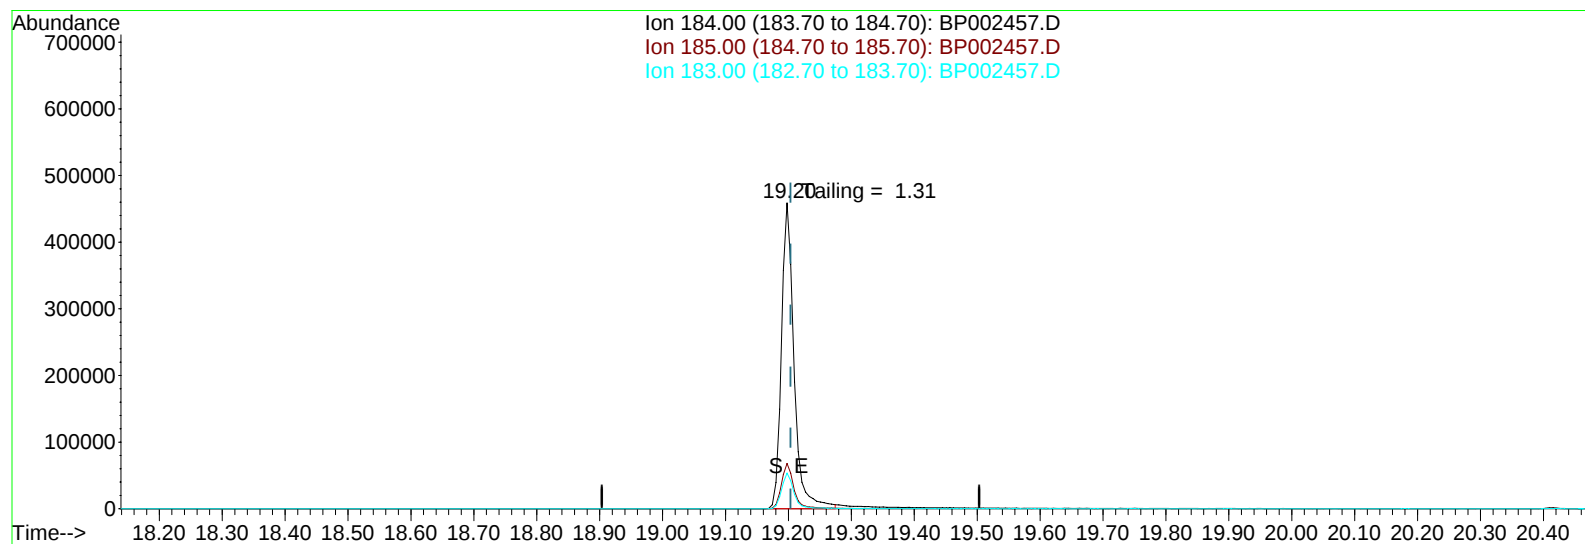

(77) Benzidine




19.198min (-0.006) 1860581.83ng

response 665196

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.81
183.00	11.50	11.66
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061920\
 Data File : BP002457.D
 Acq On : 19 Jun 2020 14:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 19:15:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

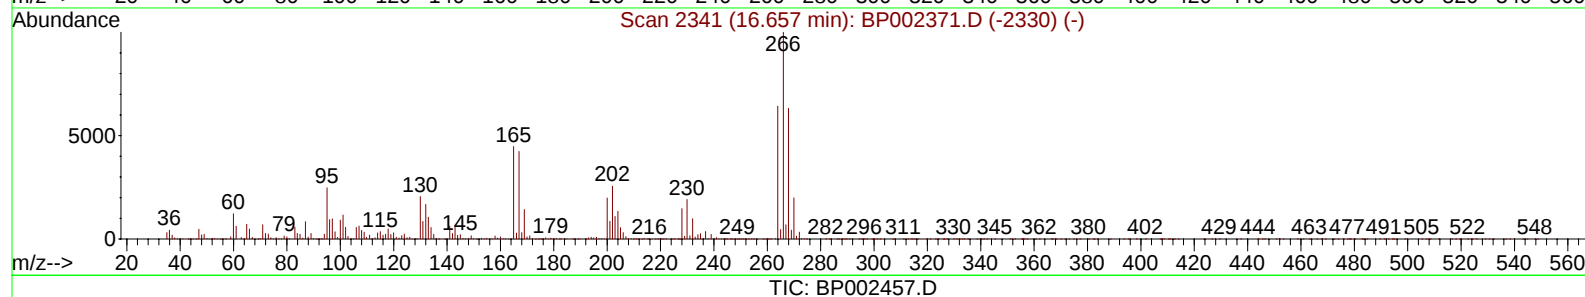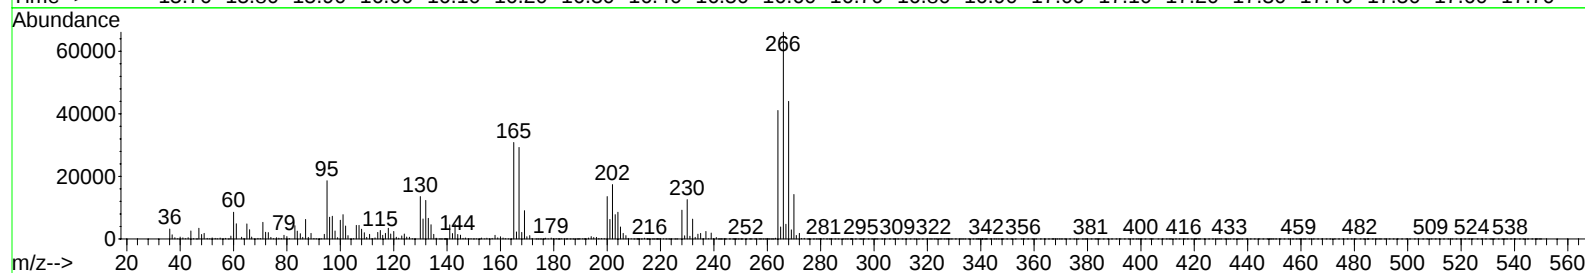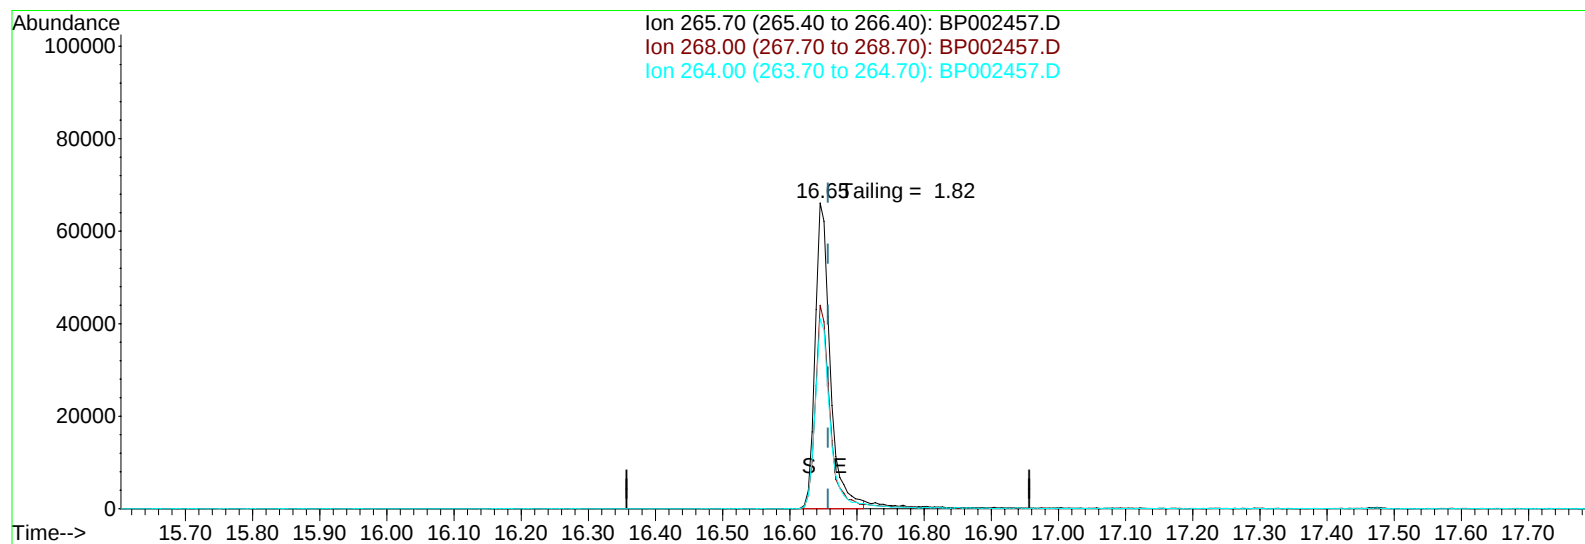

(70) Pentachlorophenol (C)

16.645min (-0.012) 1265566.35ng

response 106557

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	66.56
264.00	64.20	62.13
0.00	0.00	0.00