


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061920\
 Data File : BP002457.D
 Acq On : 19 Jun 2020 14:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

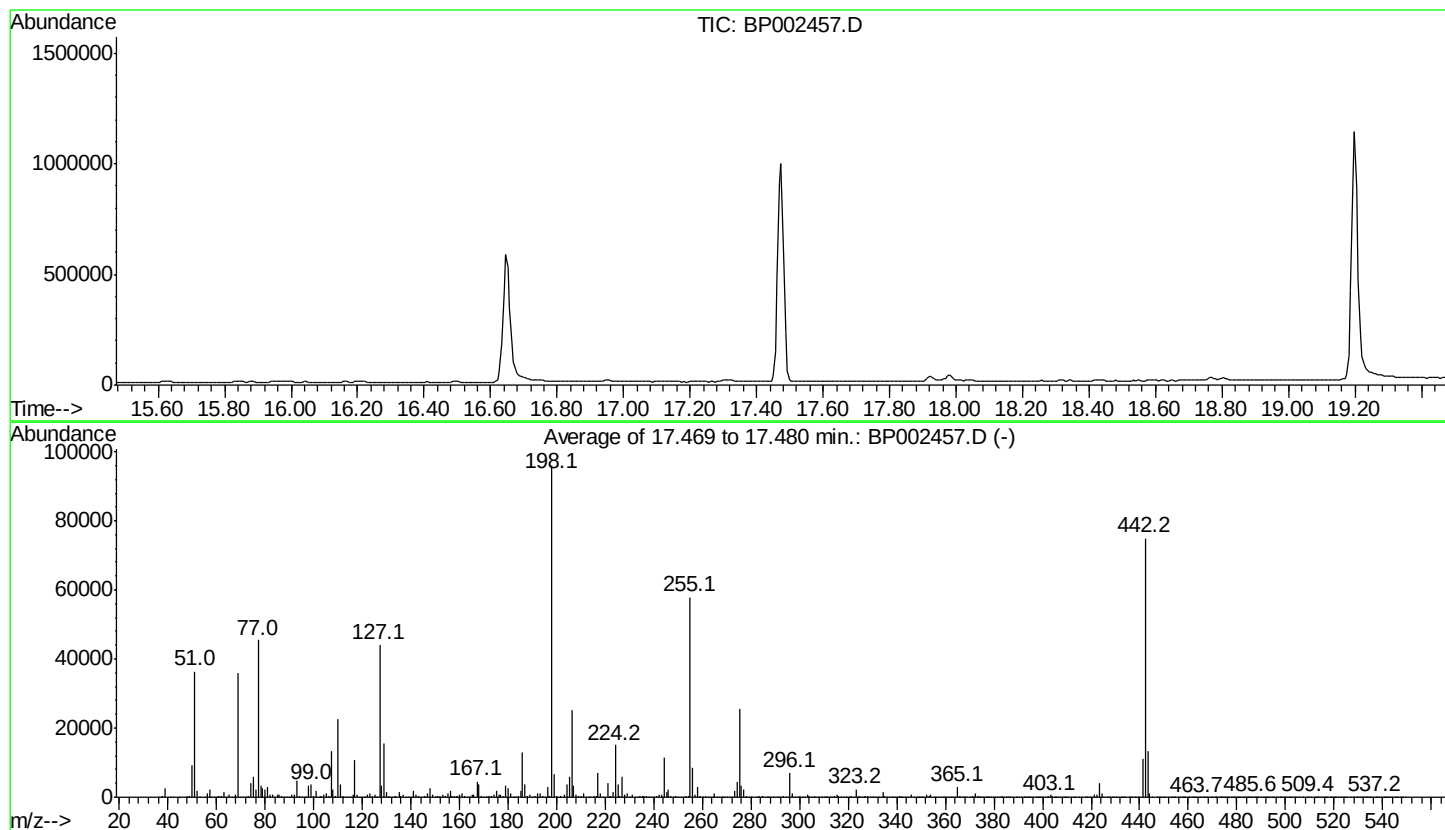

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	36368	PASS
68	69	0.00	2	1.7	611	PASS
69	198	0.00	100	37.4	35852	PASS
70	69	0.00	2	0.3	99	PASS
127	198	10	80	46.0	44152	PASS
197	198	0.00	2	0.5	457	PASS
198	198	100	100	100.0	95976	PASS
199	198	5	9	6.9	6590	PASS
275	198	10	60	26.6	25490	PASS
365	198	1	100	3.2	3091	PASS
441	198	0.01	100	11.5	11013	PASS
442	198	50	100	78.1	74934	PASS
443	442	15	24	17.8	13335	PASS