
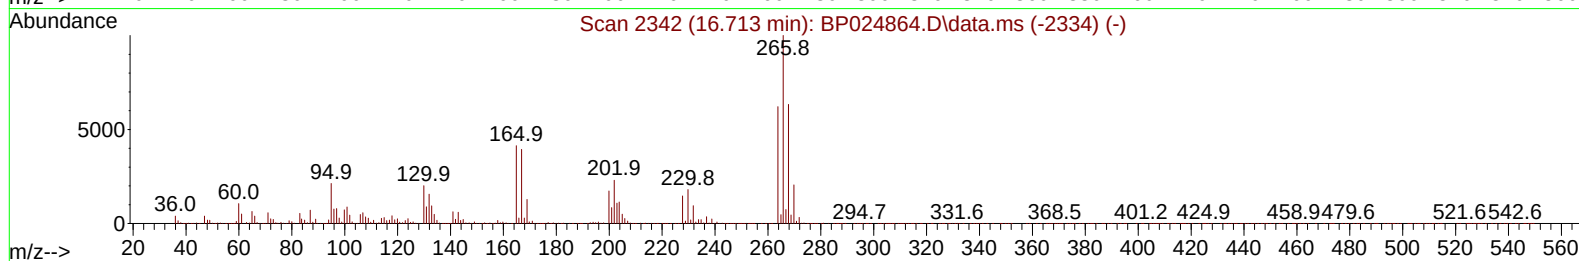
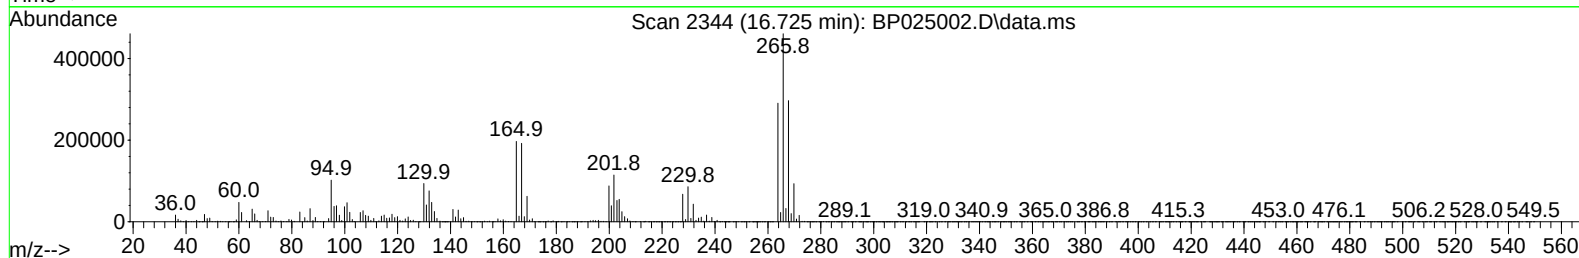


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061925\
Data File : BP025002.D
Acq On : 19 Jun 2025 14:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 14:34:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

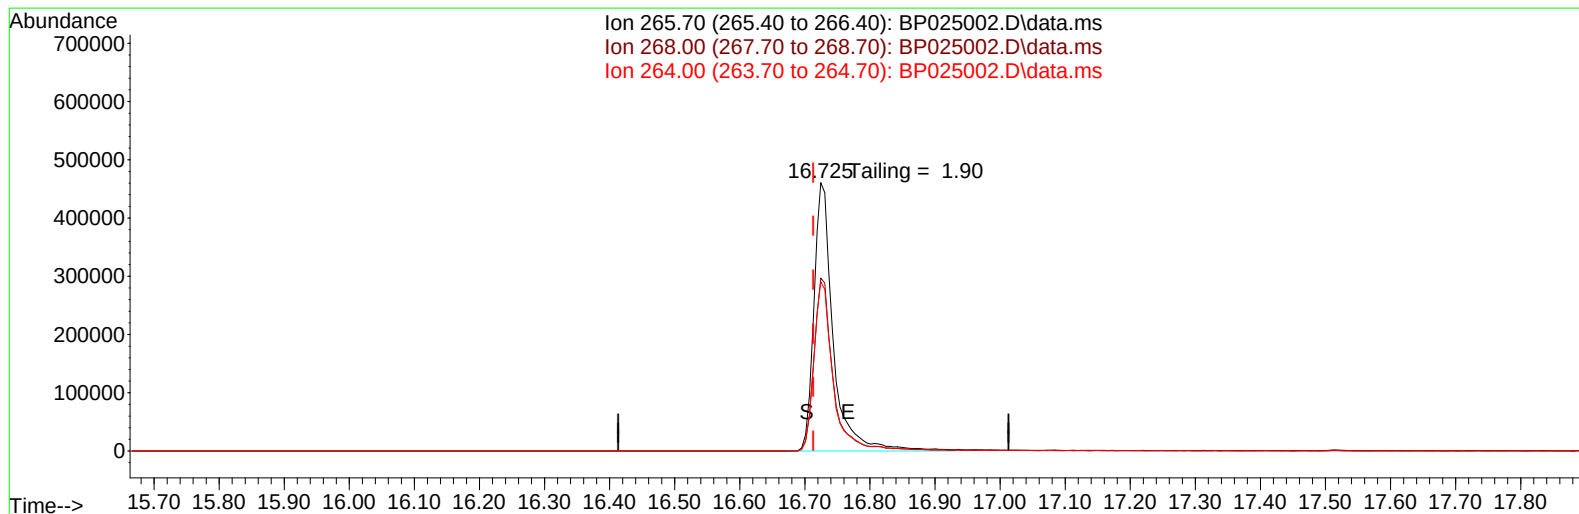

TIC: BP025002.D\data.ms

(70) Pentachlorophenol (C)




16.725min (+ 0.012) 195625.94 ng

response 947274

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.44
264.00	62.10	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061925\
Data File : BP025002.D
Acq On : 19 Jun 2025 14:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 14:34:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

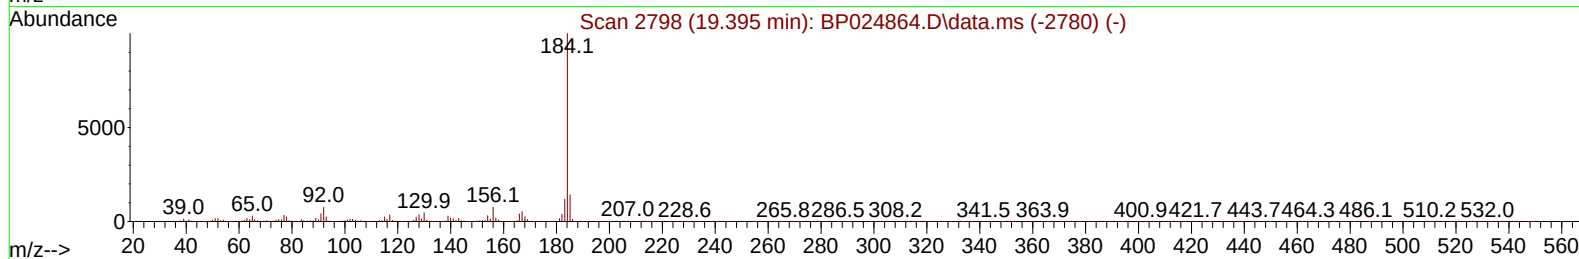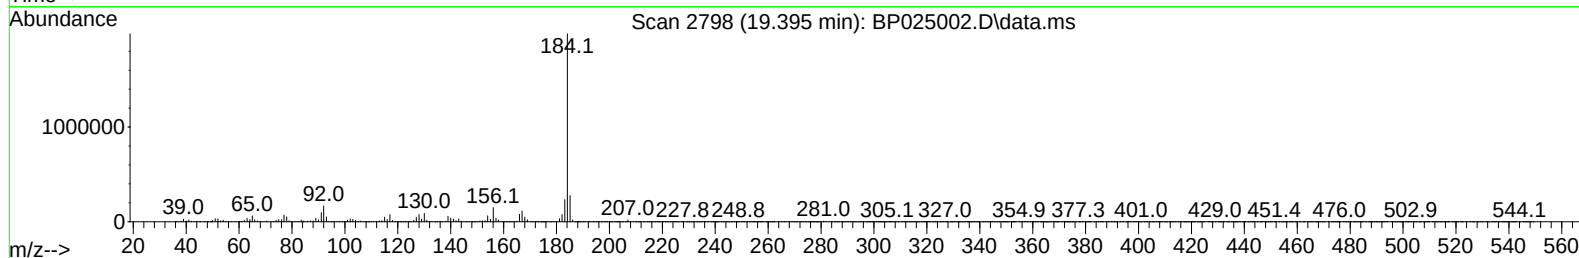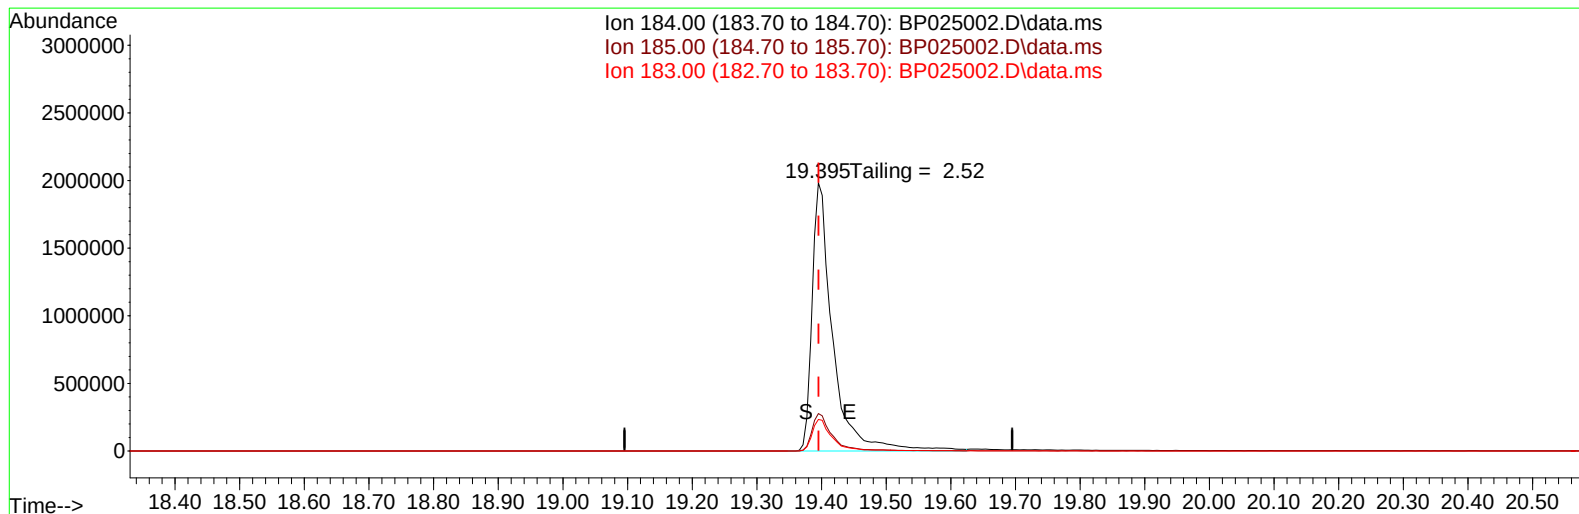

TIC: BP025002.D\data.ms

(77) Benzidine**19.395min (-0.000) 55229.69 ng****response 4348202**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.98
183.00	11.90	11.77
0.00	0.00	0.00