
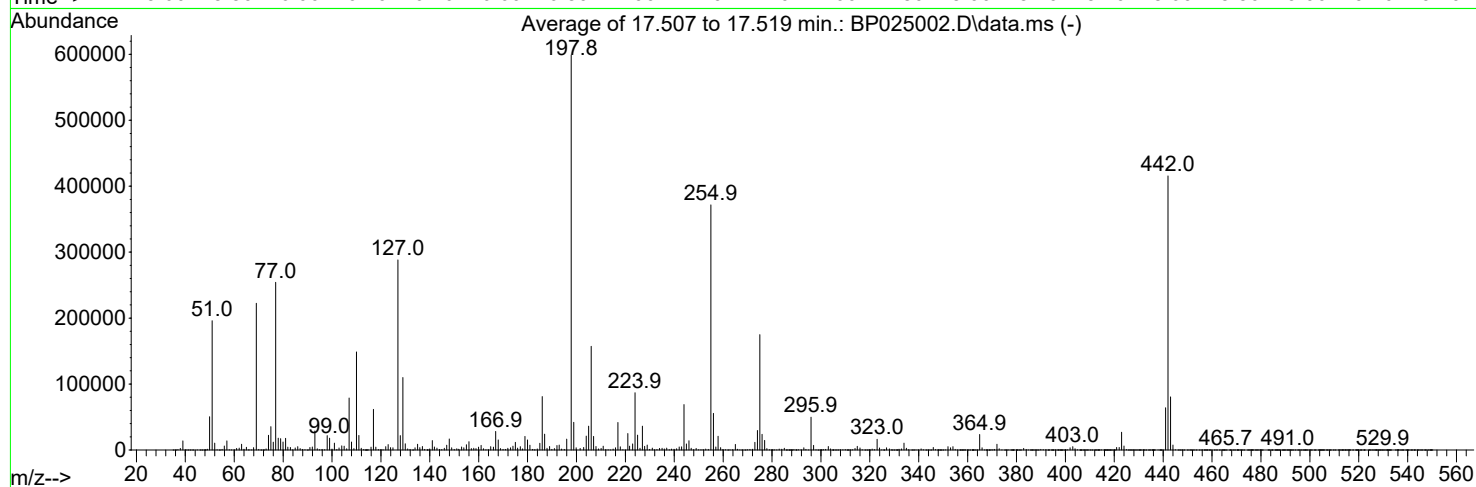


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061925\
Data File : BP025002.D
Acq On : 19 Jun 2025 14:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 06 16:20:27 2025

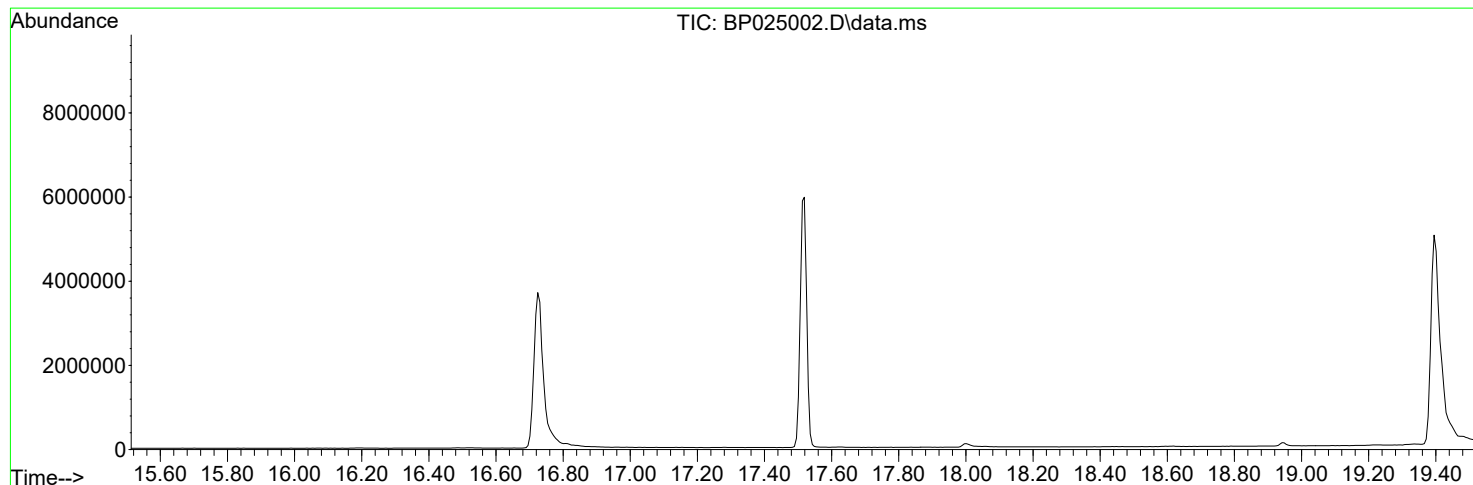

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	3697	PASS
69	69	100	100	100.0	222599	PASS
70	69	0.00	2	0.4	991	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	598687	PASS
199	198	5	9	7.0	42099	PASS
365	198	1	100	3.9	23634	PASS
441	443	0.01	150	79.6	64086	PASS
442	442	100	100	100.0	415552	PASS
443	442	15	24	19.4	80507	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/19/2025	BNA_P	<u>BP025002.D</u>
Compound Name	Response	Retention Time
DDT	2218256	20.677
DDD	76284	20.224
DDE	7763	19.689
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
84047	2302303	3.65

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061925\
Data File : BP025002.D
Acq On : 19 Jun 2025 14:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 19 14:34:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

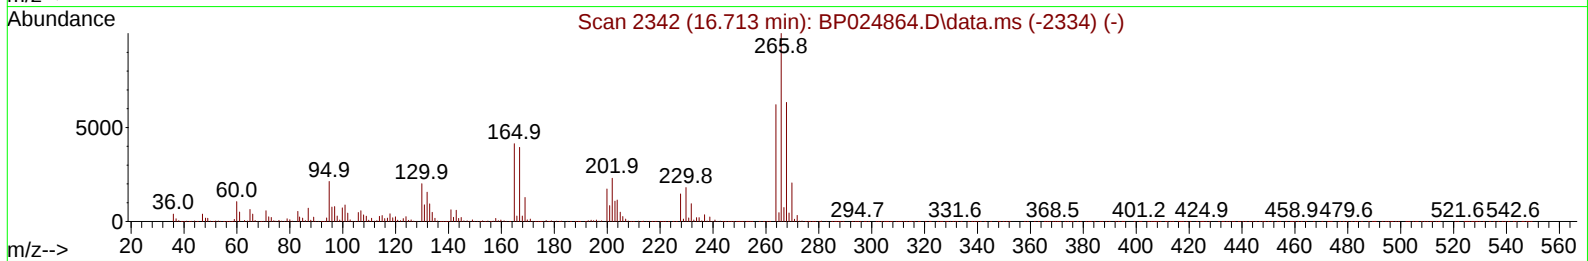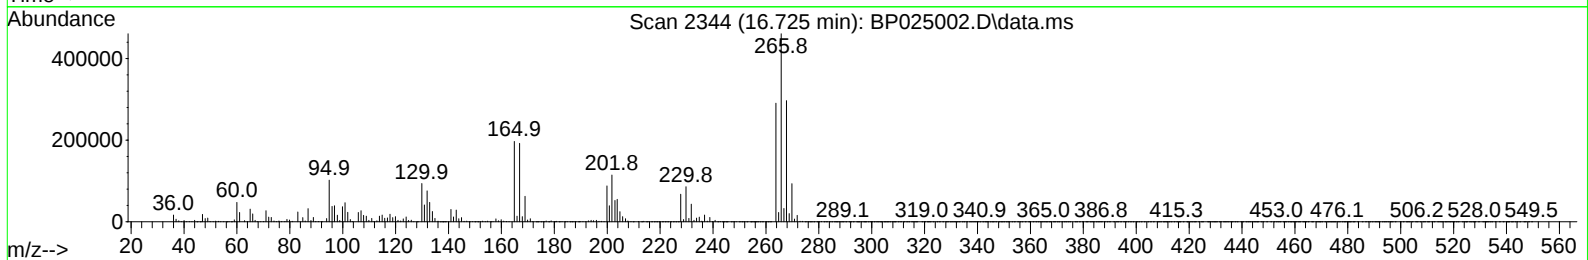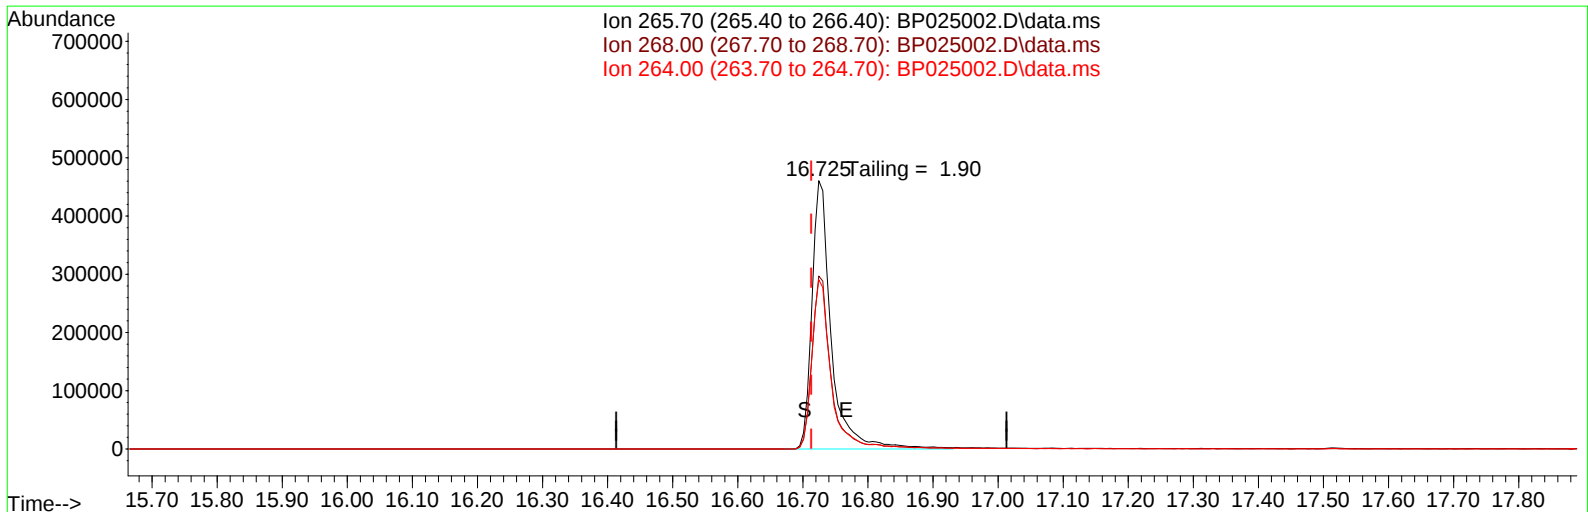

TIC: BP025002.D\data.ms

(70) Pentachlorophenol (C)

16.725min (+ 0.012) 195625.94 ng




response 947274

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.44
264.00	62.10	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061925\
Data File : BP025002.D
Acq On : 19 Jun 2025 14:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 19 14:34:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

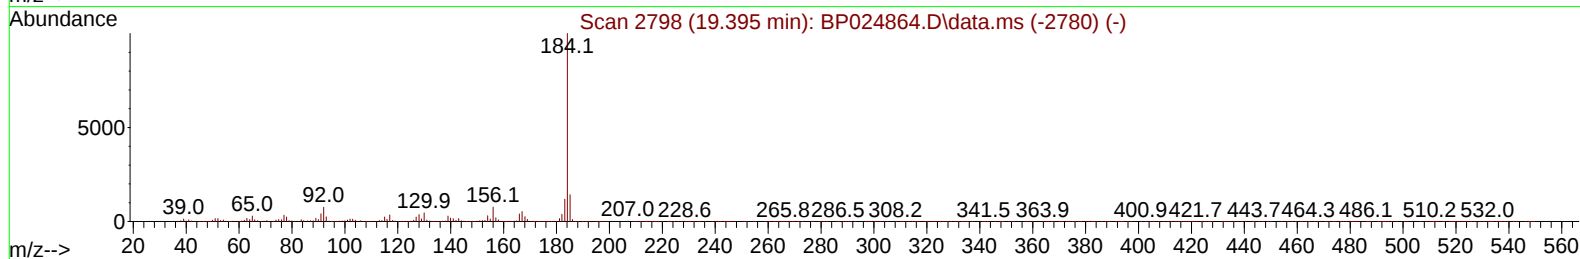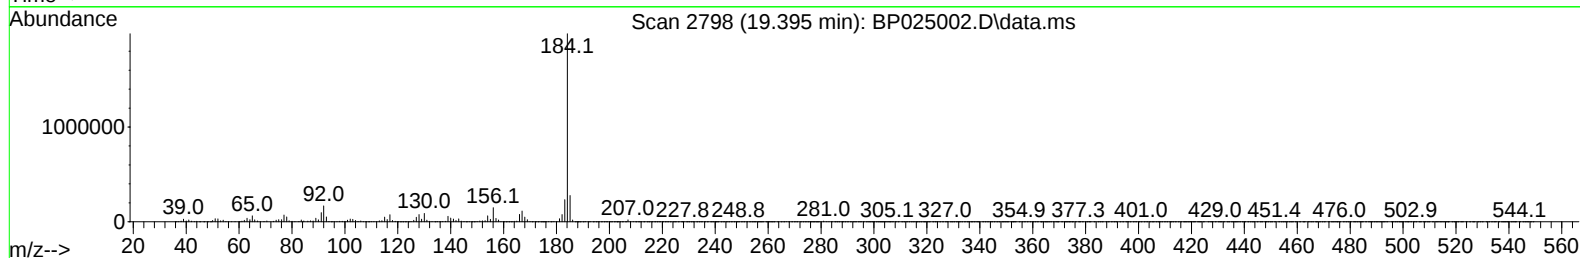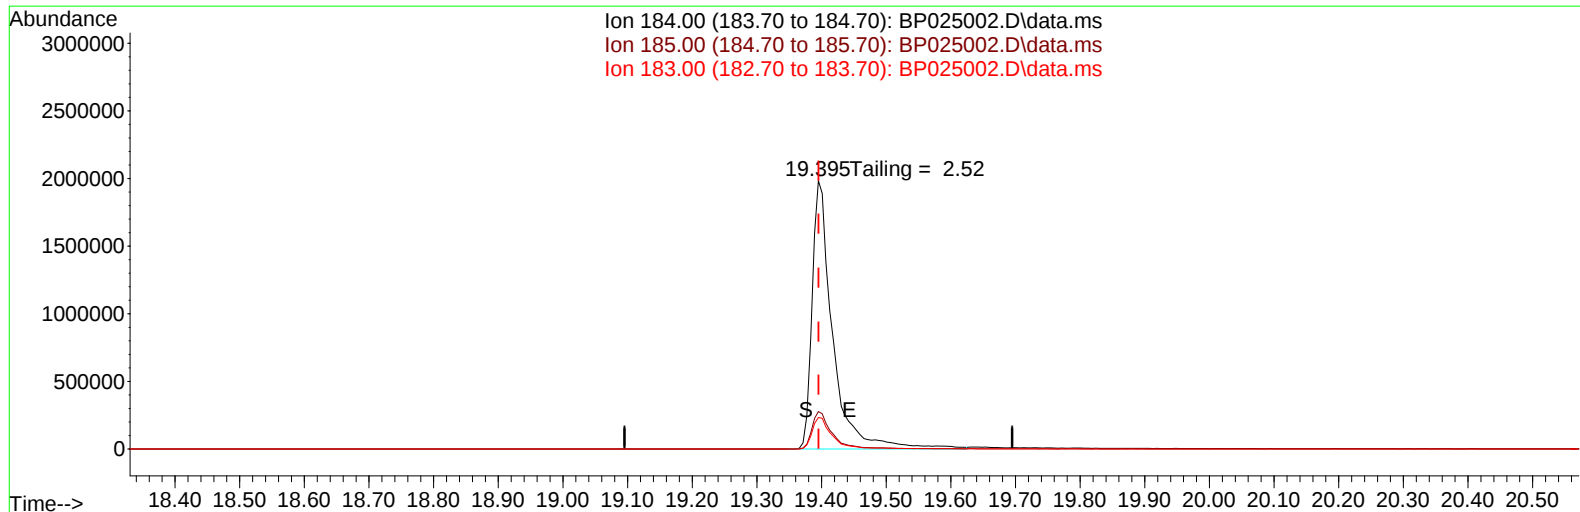

TIC: BP025002.D\data.ms

(77) Benzidine

19.395min (-0.000) 55229.69 ng

response 4348202

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.98
183.00	11.90	11.77
0.00	0.00	0.00