

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010770.D
 Acq On : 20 Jun 2022 20:13
 Operator : CG/JU
 Sample : N3358-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4S0

Quant Time: Jun 21 00:46:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	115911	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	438674	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	283586	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	613473	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	683514	20.000	ng/ul	0.00
88) Perylene-d12	23.692	264	799914	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	13791	5.114	ng/uL	0.00
4) Pyridine-d5	3.705	84	81628	11.638	ng/ul	0.01
7) Phenol-d5	6.999	99	62955	7.485	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	182152	35.570	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	202210	28.248	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	125377	18.449	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	121478	37.297	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	580	0.166	ng/ul	0.11
28) 2,4-Dichlorophenol-d3	10.246	165	213027	32.948	ng/ul	0.00
31) 4-Chloroaniline-d4	10.757	131	270468	29.698	ng/ul	0.00
46) Dimethylphthalate-d6	13.869	166	804748	41.333	ng/ul	0.00
49) Acenaphthylene-d8	14.145	160	921779	39.093	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	53	0.018	ng/ul	0.00
60) Fluorene-d10	15.451	176	719019	41.546	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.586	200	113069	30.892	ng/ul	0.00
73) Anthracene-d10	17.310	188	1171842	42.121	ng/ul	0.00
81) Pyrene-d10	19.551	212	1466518	43.159	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	1671470	41.964	ng/ul	0.00


Target Compounds					Qvalue
35) 4-Chloro-3-methylphenol	11.963	107	240216	38.094 ng/ul#	22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010770.D
Acq On : 20 Jun 2022 20:13
Operator : CG/JU
Sample : N3358-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4S0

Quant Time: Jun 21 00:46:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 16:18:42 2022
Response via : Initial Calibration

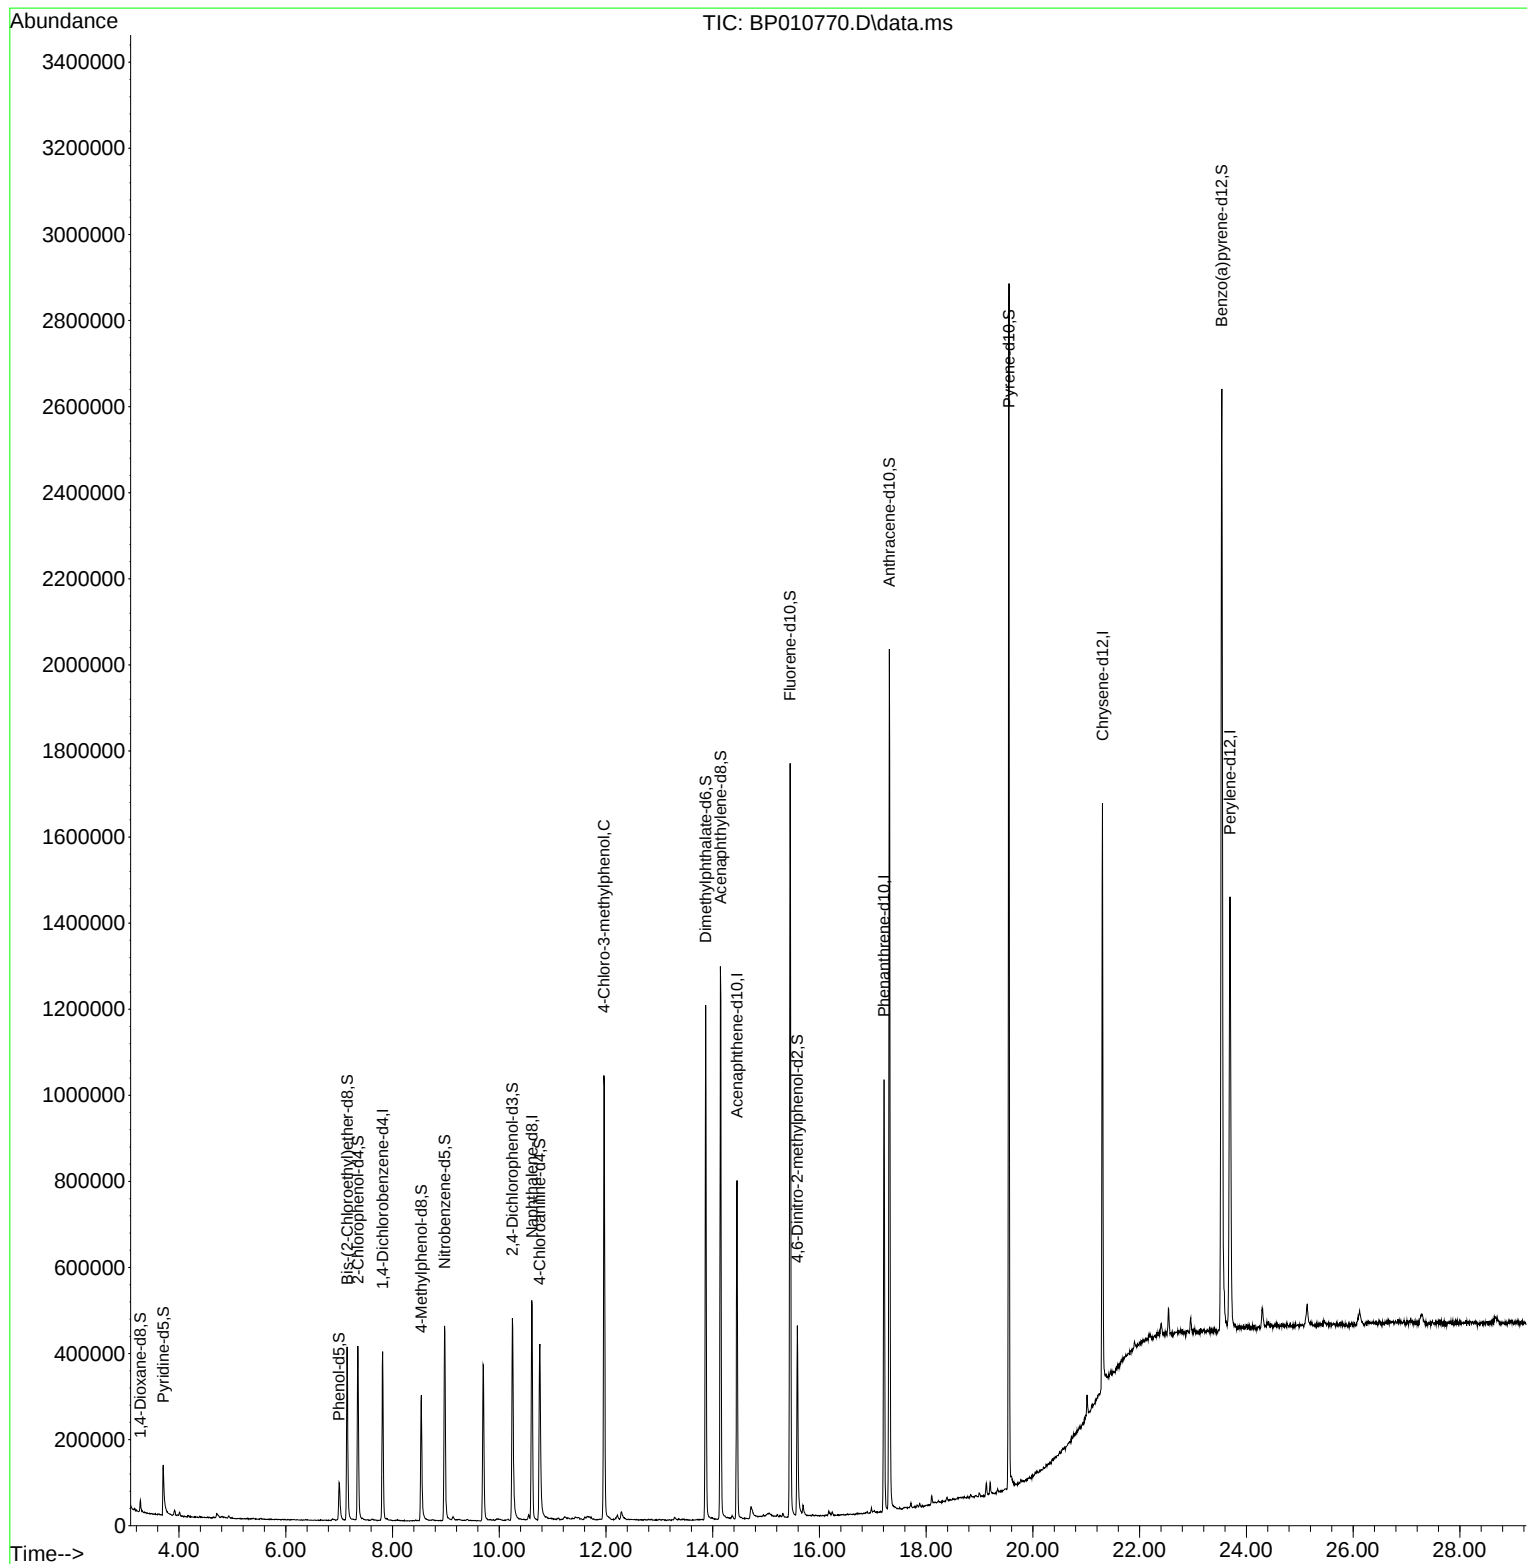

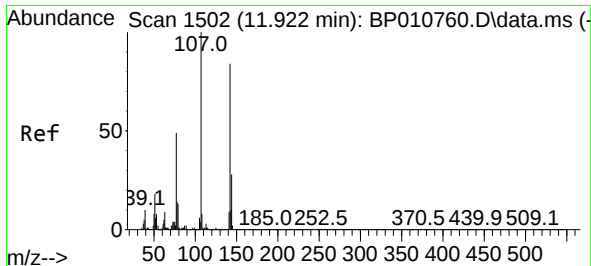

#35
 4-Chloro-3-methylphenol
 Concen: 38.094 ng/ul
 RT: 11.963 min Scan# 11
 Delta R.T. 0.041 min
 Lab File: BP010770.D
 Acq: 20 Jun 2022 20:13

Instrument :
 BNA_P
 ClientSampleId :
 EW4S0

Tgt Ion:107 Resp: 240216
 Ion Ratio Lower Upper
 107 100
 144 0.1 18.6 27.8#
 142 0.0 59.6 89.4#

