




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010767.D
Acq On : 20 Jun 2022 18:32
Operator : CG/JU
Sample : N3358-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4R8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 00:46:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 16:18:42 2022
Response via : Initial Calibration

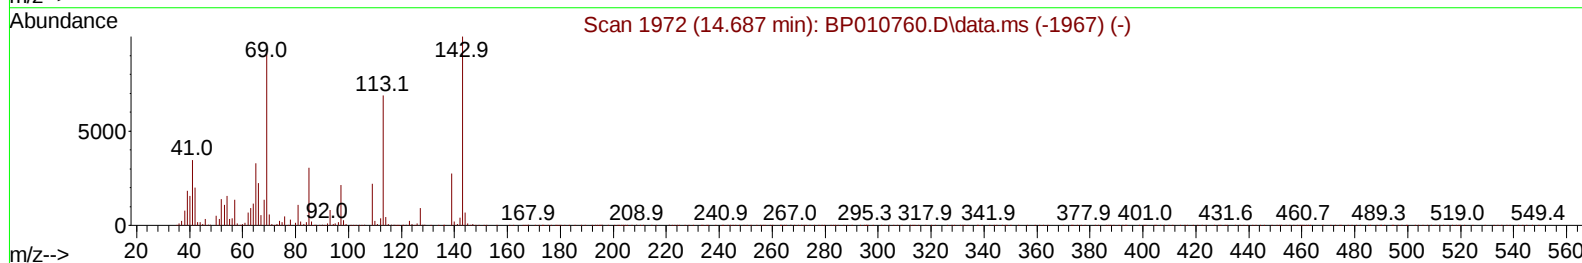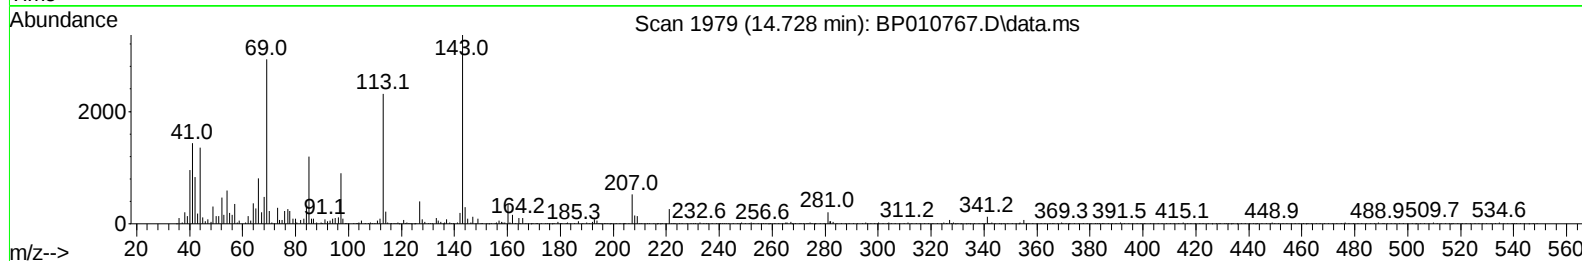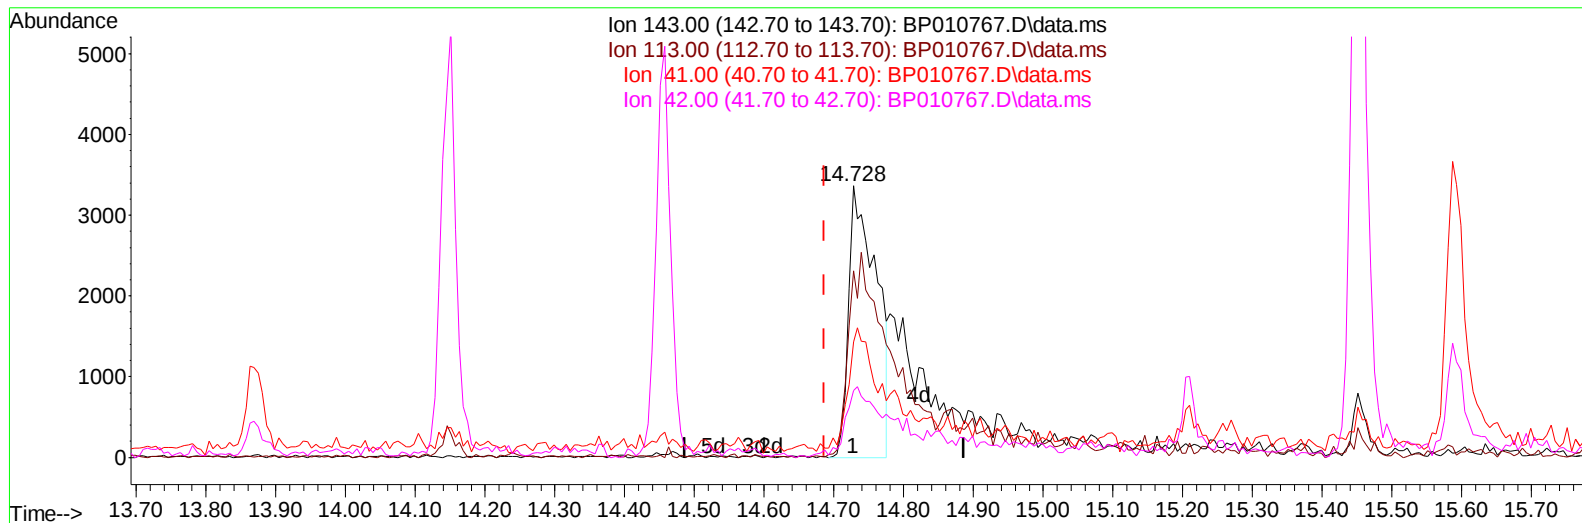

TIC: BP010767.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.728min (+ 0.041) 3.17 ng/ul

response 9194

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	68.68#
41.00	59.00	42.56#
42.00	41.10	24.75#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010767.D
Acq On : 20 Jun 2022 18:32
Operator : CG/JU
Sample : N3358-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4R8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 00:46:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 16:18:42 2022
Response via : Initial Calibration

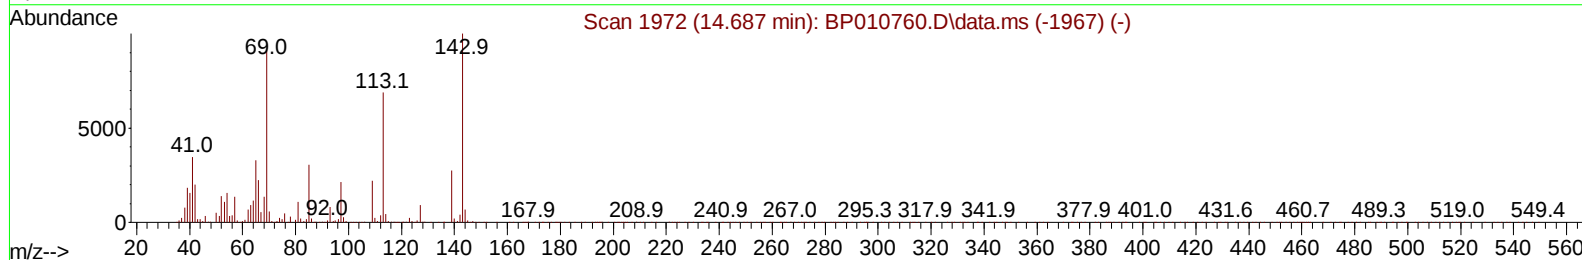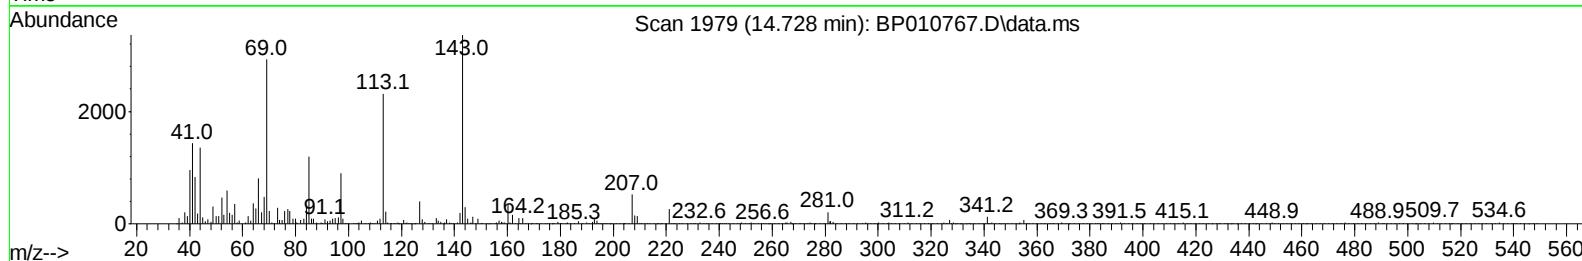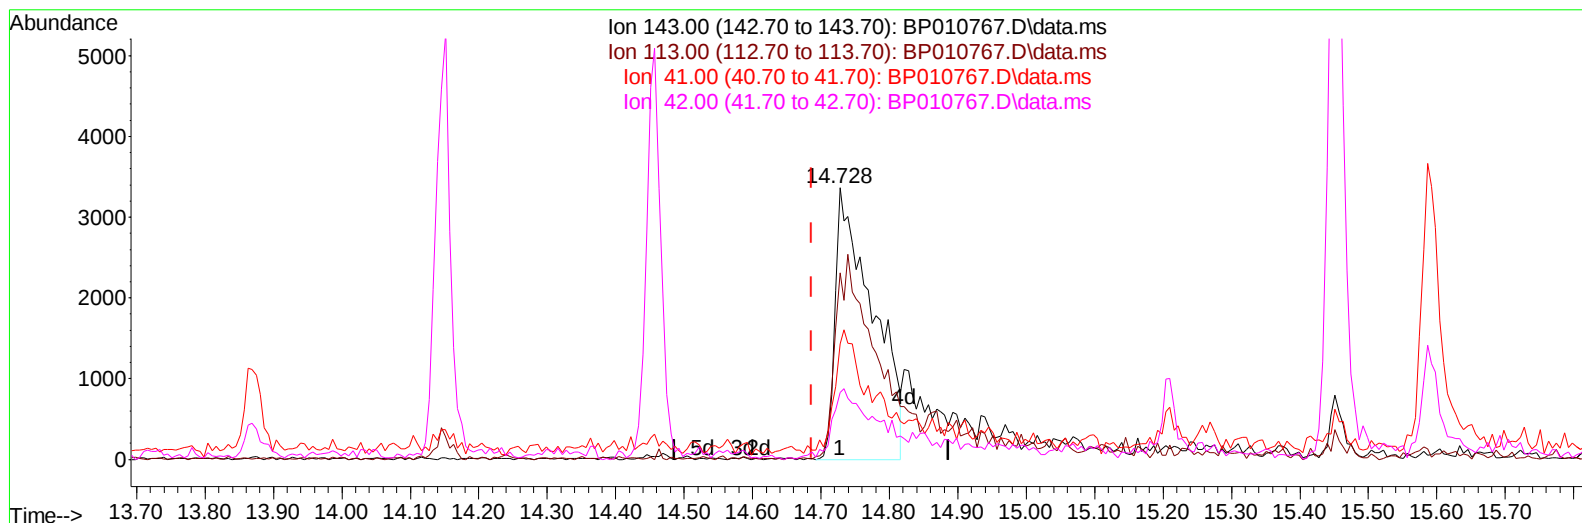

TIC: BP010767.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.728min (+ 0.041) 4.37 ng/ul m

response 12688

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	68.68#
41.00	59.00	42.56#
42.00	41.10	24.75#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010767.D
 Acq On : 20 Jun 2022 18:32
 Operator : CG/JU
 Sample : N3358-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4R8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 00:46:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

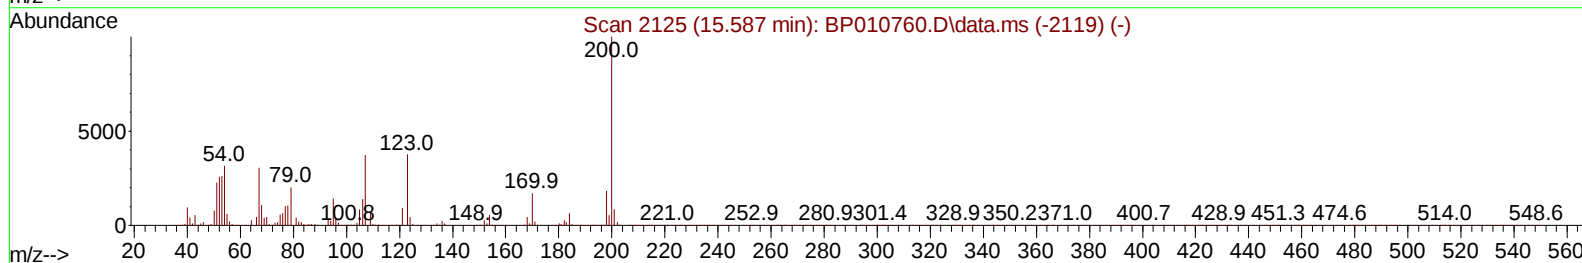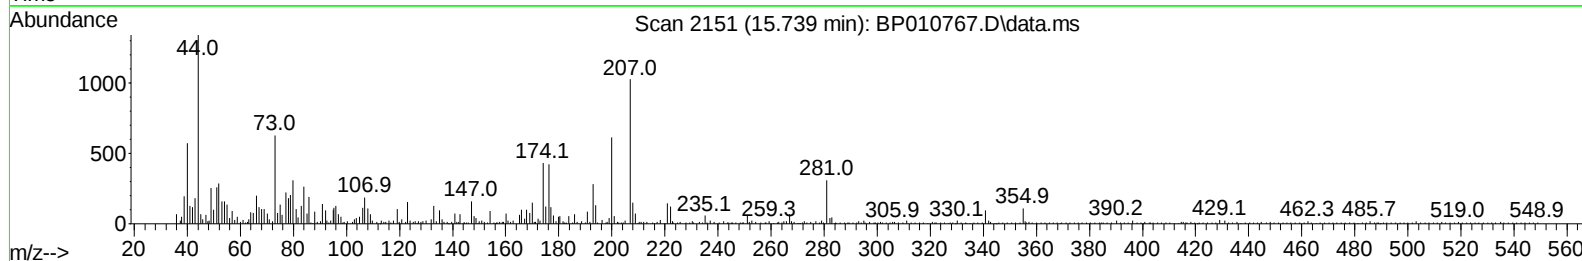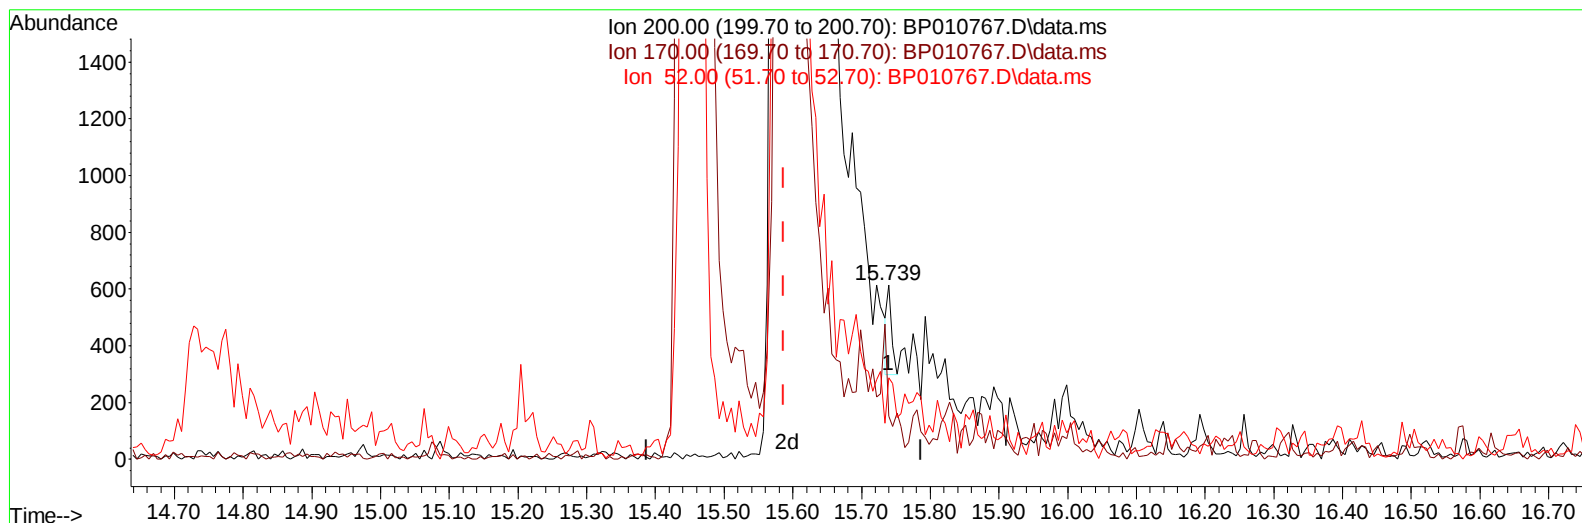

TIC: BP010767.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.739min (+ 0.153) 0.04 ng/ul

response 148

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.60	24.72
52.00	57.40	46.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010767.D
 Acq On : 20 Jun 2022 18:32
 Operator : CG/JU
 Sample : N3358-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4R8

Manual IntegrationsAPPROVED

Quant Time: Jun 21 00:46:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

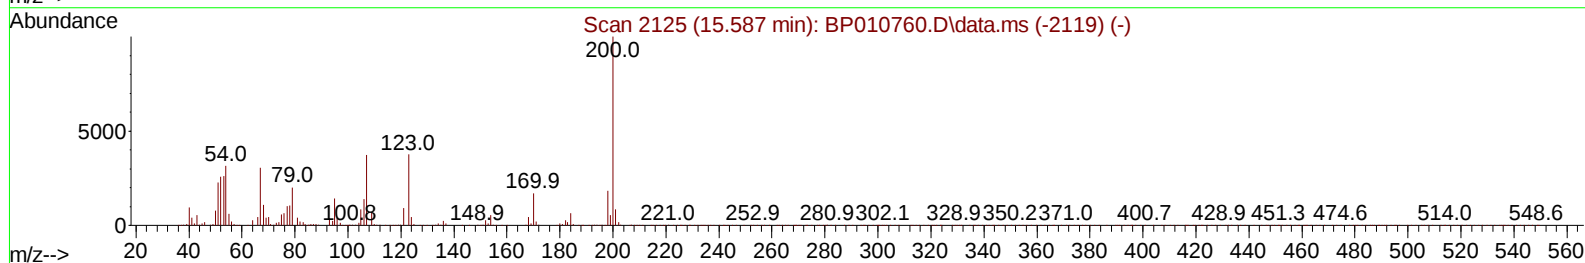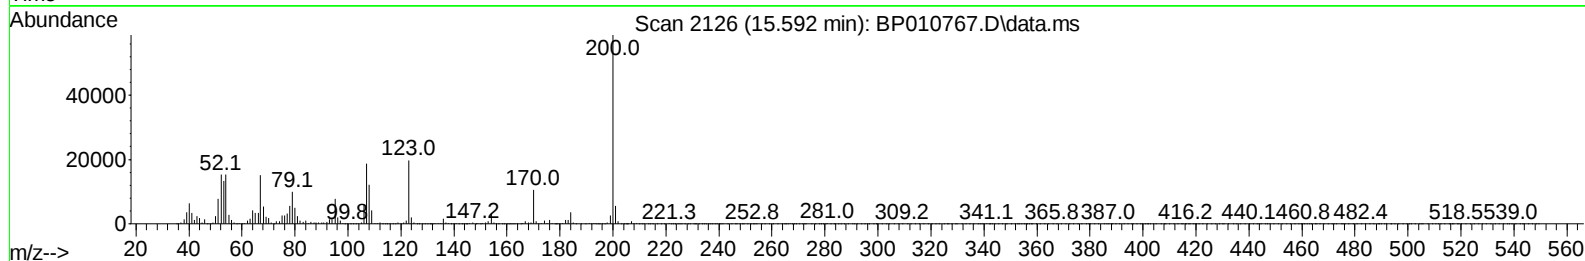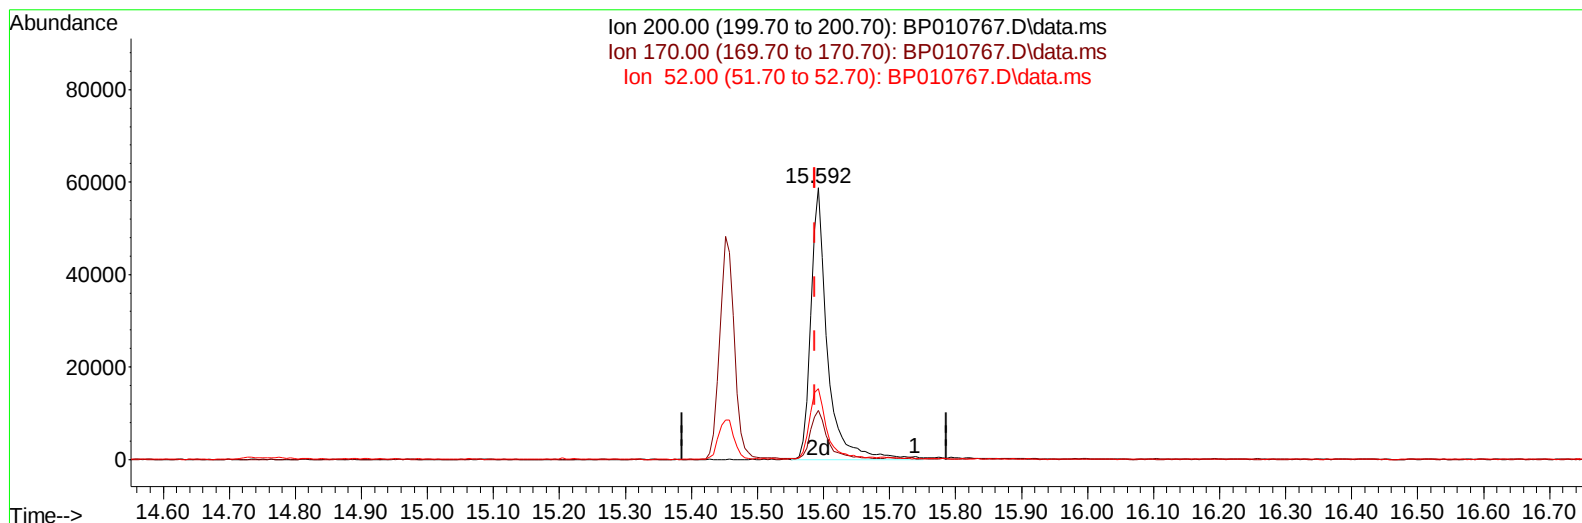

TIC: BP010767.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.592min (+ 0.006) 29.38 ng/ul m

response 102820

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.60	18.01#
52.00	57.40	26.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010767.D
 Acq On : 20 Jun 2022 18:32
 Operator : CG/JU
 Sample : N3358-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4R8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 00:46:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	125779	20.000	ng/ul	0.00
20) Naphthalene-d8	10.616	136	474104	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	286190	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	586568	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	640155	20.000	ng/ul	0.00
88) Perylene-d12	23.698	264	720172	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	16123	5.509	ng/uL	0.00
4) Pyridine-d5	3.705	84	66009	8.673	ng/ul	0.01
7) Phenol-d5	6.999	99	61305	6.717	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	174232	31.354	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	193209	24.873	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	114736	15.559	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	112826	32.052	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	115186	30.543	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	181922	26.035	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	250478	25.448	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	725602	36.929	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	785283	33.001	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	12688m	4.371	ng/ul	0.04
60) Fluorene-d10	15.451	176	645154	36.939	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	102820m	29.380	ng/ul	0.00
73) Anthracene-d10	17.310	188	1108156	41.659	ng/ul	0.00
81) Pyrene-d10	19.551	212	1363828	42.856	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.545	264	1512548	42.178	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010767.D
Acq On : 20 Jun 2022 18:32
Operator : CG/JU
Sample : N3358-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4R8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 00:46:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 16:18:42 2022
Response via : Initial Calibration

