




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010768.D
 Acq On : 20 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3358-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4S1

Manual IntegrationsAPPROVED

Quant Time: Jun 21 00:46:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

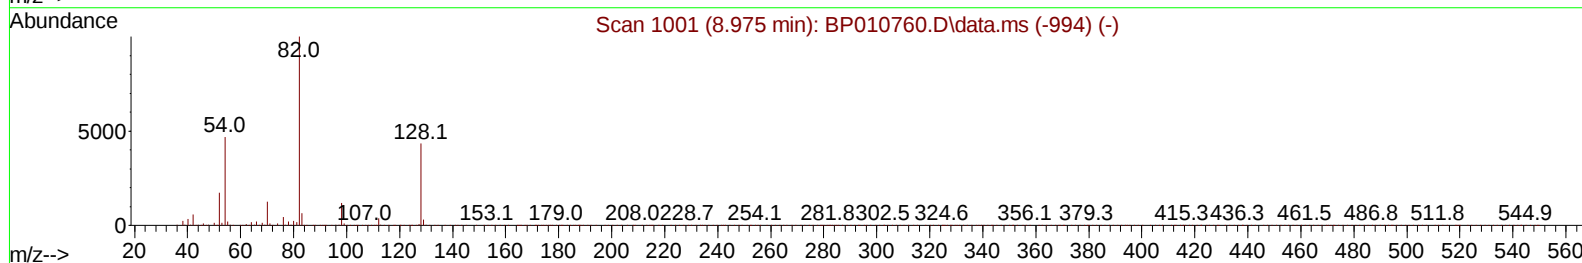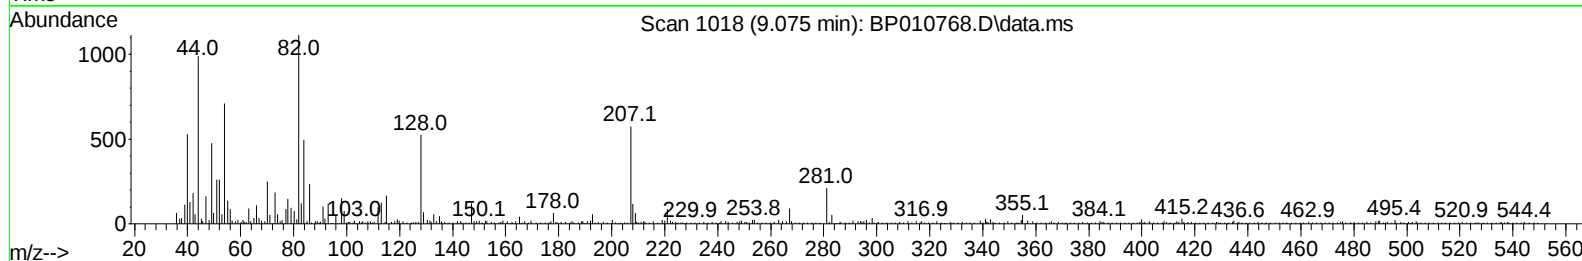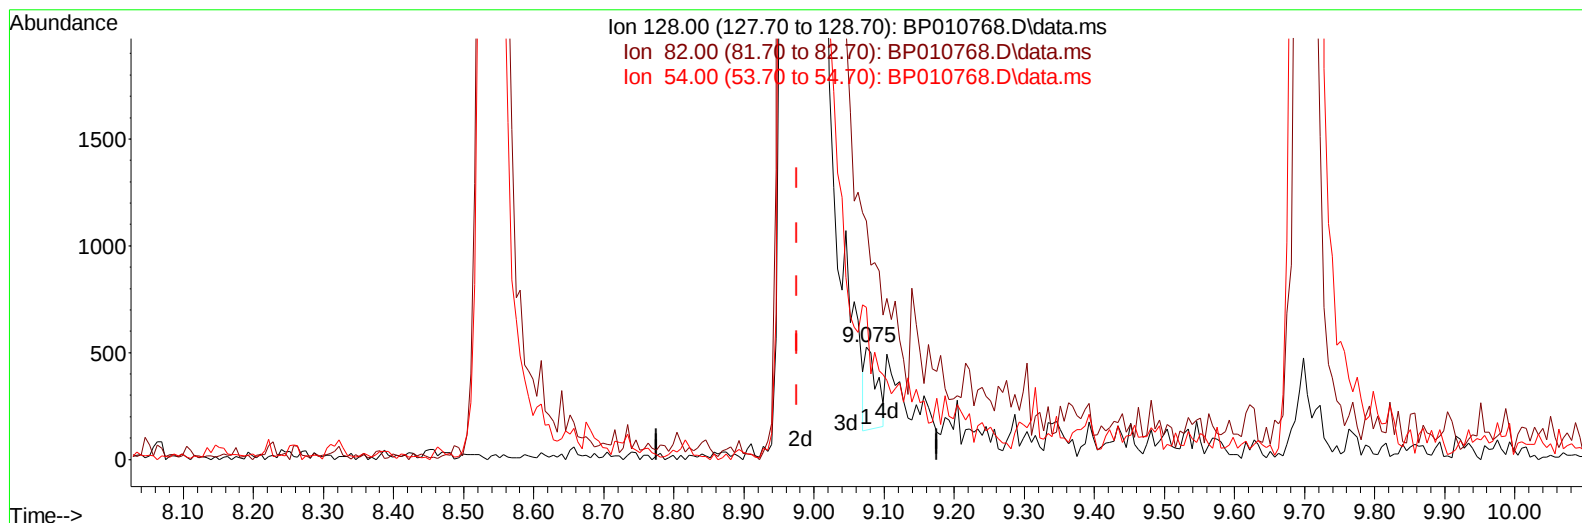

TIC: BP010768.D\data.ms

(21) Nitrobenzene-d5 (S)

9.075min (+ 0.100) 0.13 ng/u1

response 450

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	249.70	211.57
54.00	155.90	134.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010768.D
Acq On : 20 Jun 2022 19:06
Operator : CG/JU
Sample : N3358-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4S1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 00:46:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 16:18:42 2022
Response via : Initial Calibration

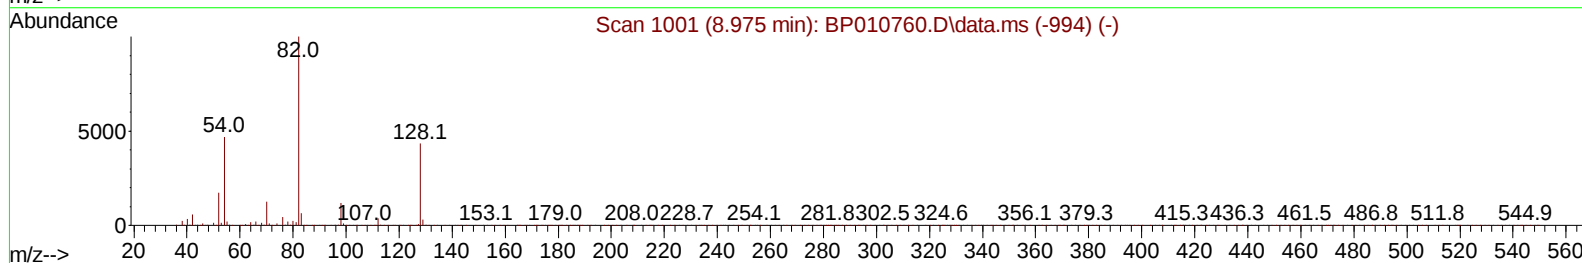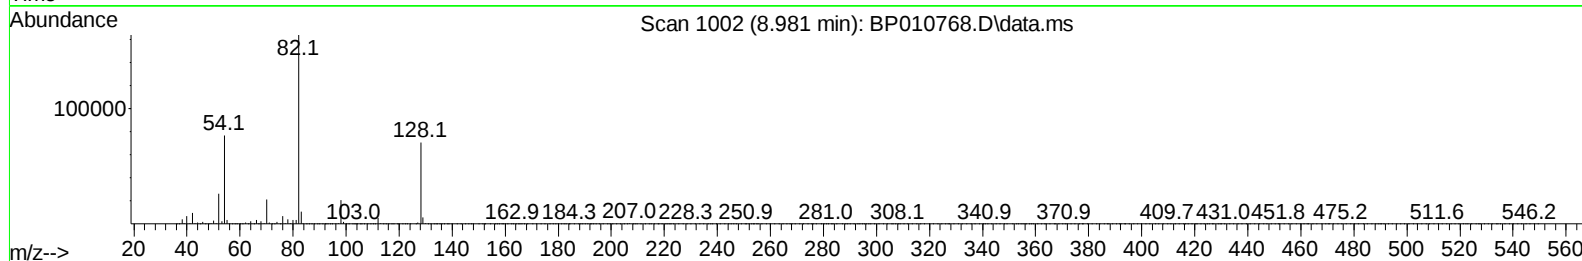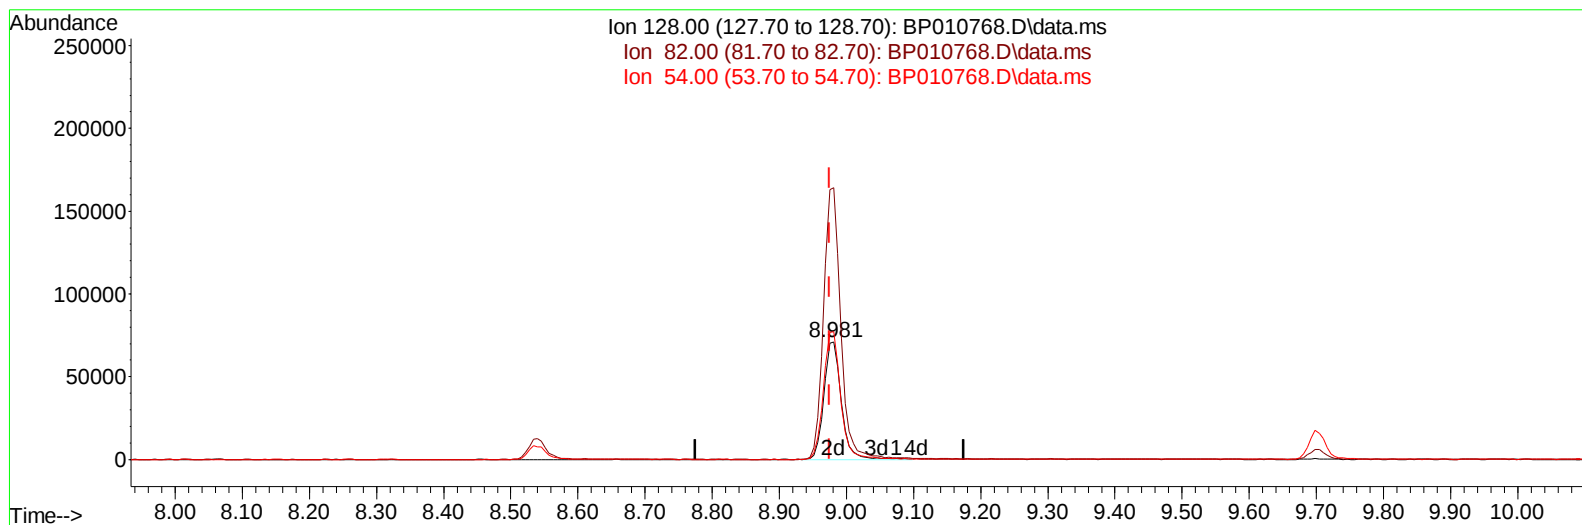

TIC: BP010768.D\data.ms

(21) Nitrobenzene-d5 (S)

8.981min (+ 0.005) 37.60 ng/ul m

response 127619

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	249.70	231.63
54.00	155.90	108.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010768.D
 Acq On : 20 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3358-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4S1

Manual IntegrationsAPPROVED

Quant Time: Jun 21 00:46:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

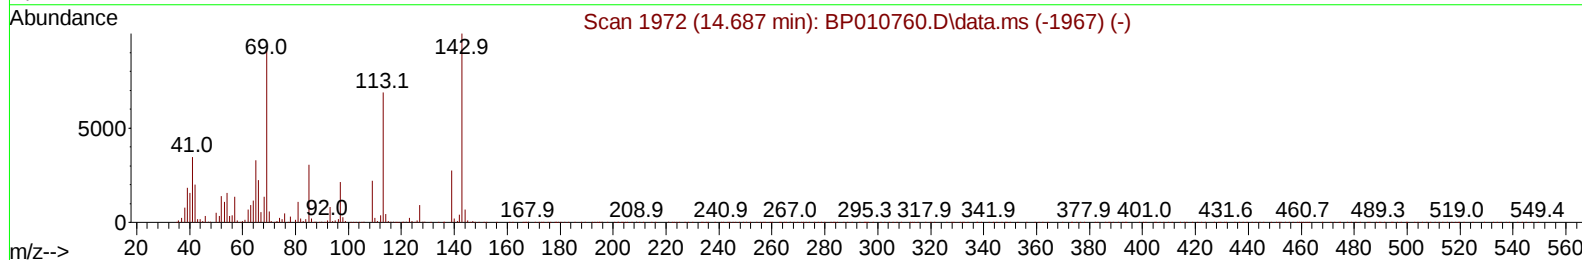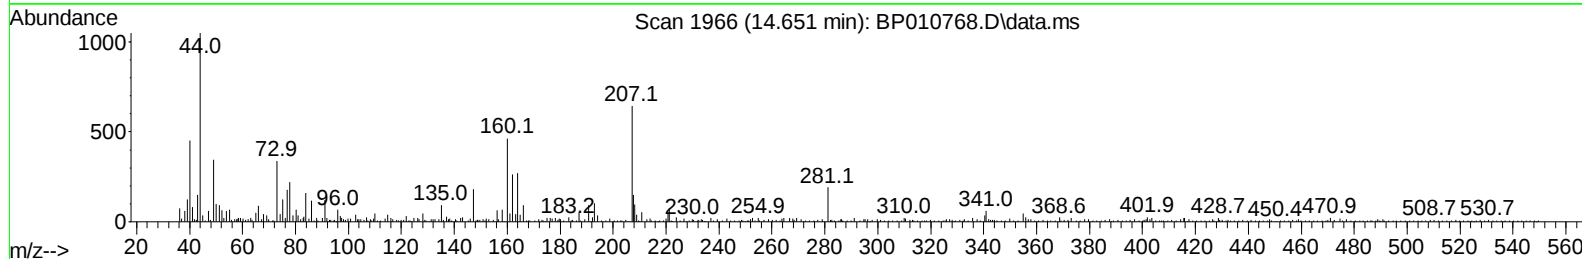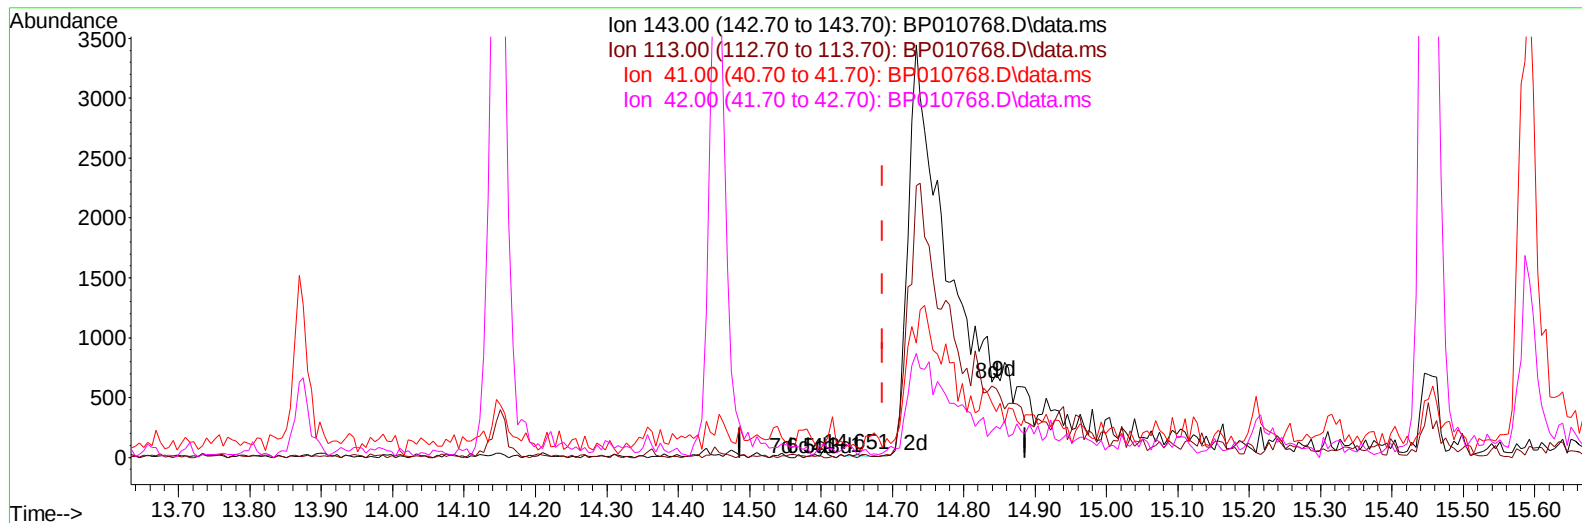

TIC: BP010768.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.651min (-0.036) 0.01 ng/u1

response 19

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	0.00#
41.00	59.00	324.00#
42.00	41.10	104.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010768.D
 Acq On : 20 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3358-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4S1

Manual IntegrationsAPPROVED

Quant Time: Jun 21 00:46:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

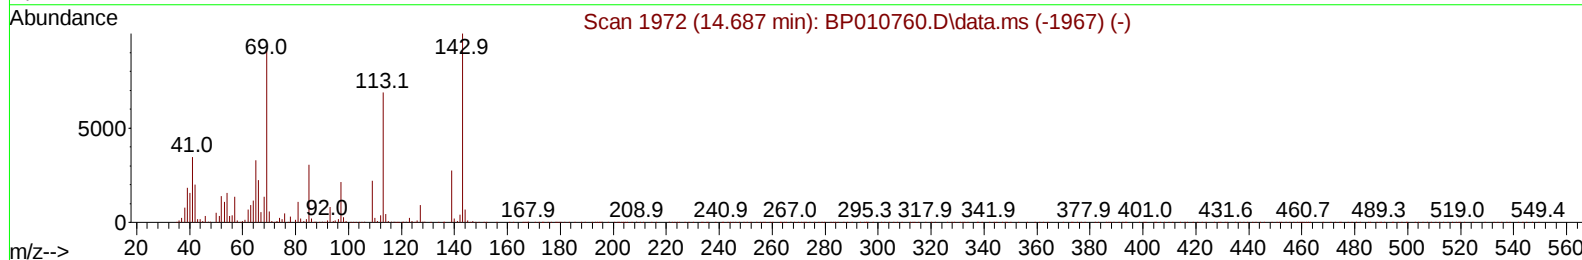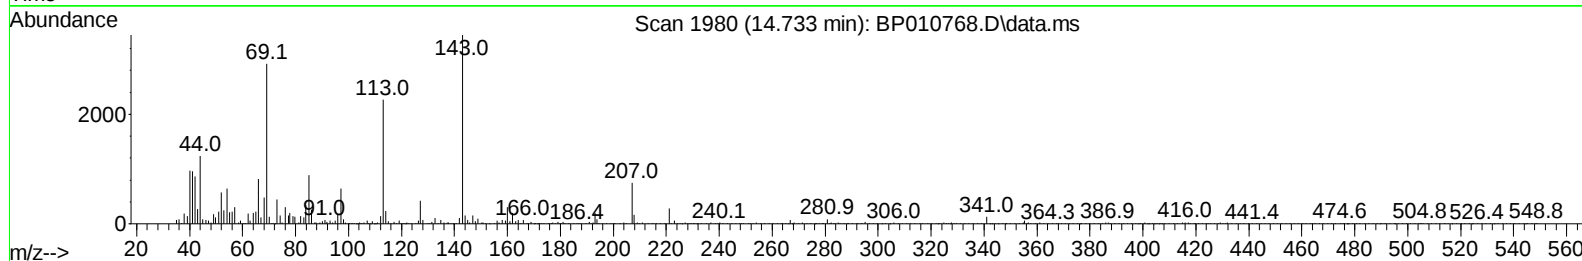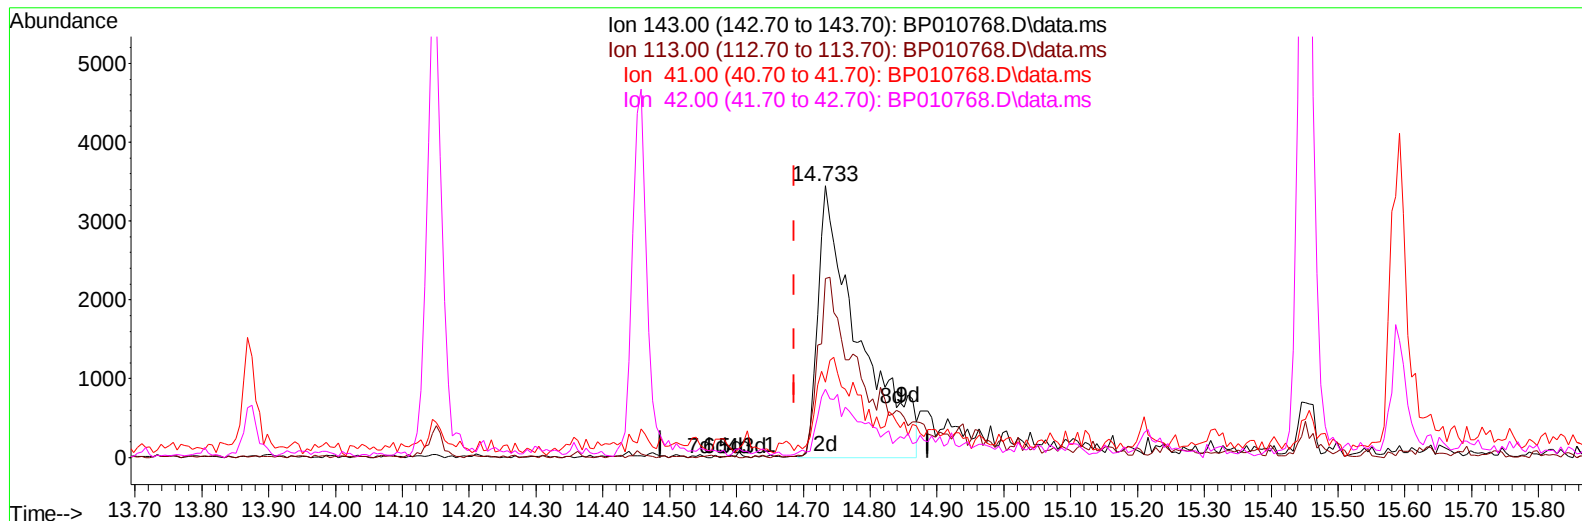

TIC: BP010768.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.733min (+ 0.047) 5.24 ng/ul m

response 14549

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	65.83#
41.00	59.00	27.72#
42.00	41.10	25.20#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010768.D
Acq On : 20 Jun 2022 19:06
Operator : CG/JU
Sample : N3358-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4S1

Manual IntegrationsAPPROVED

Quant Time: Jun 21 00:46:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 16:18:42 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :mohammad ahmed 06/27/2022

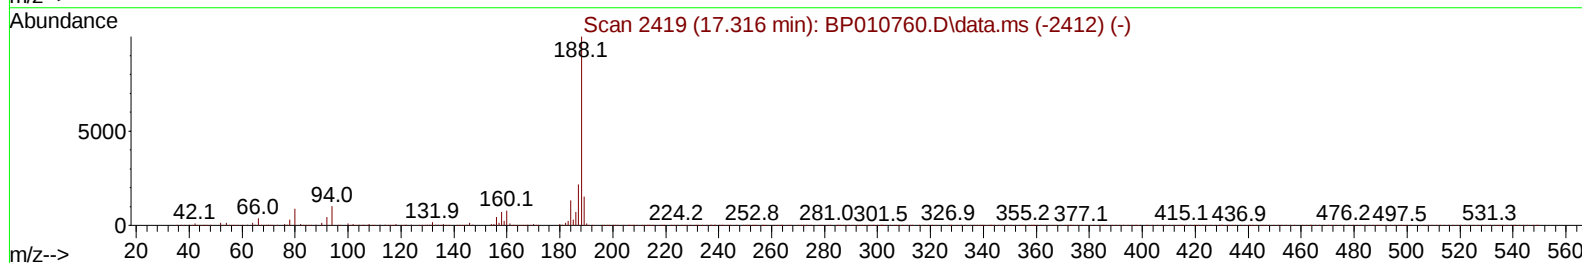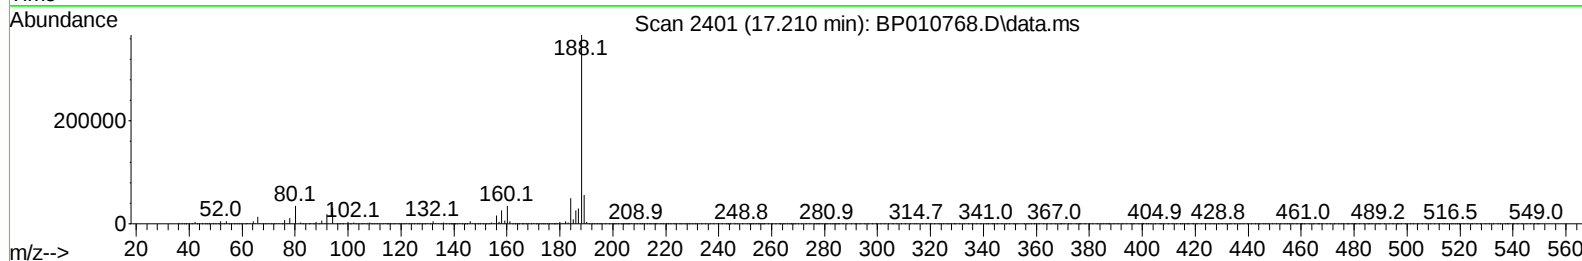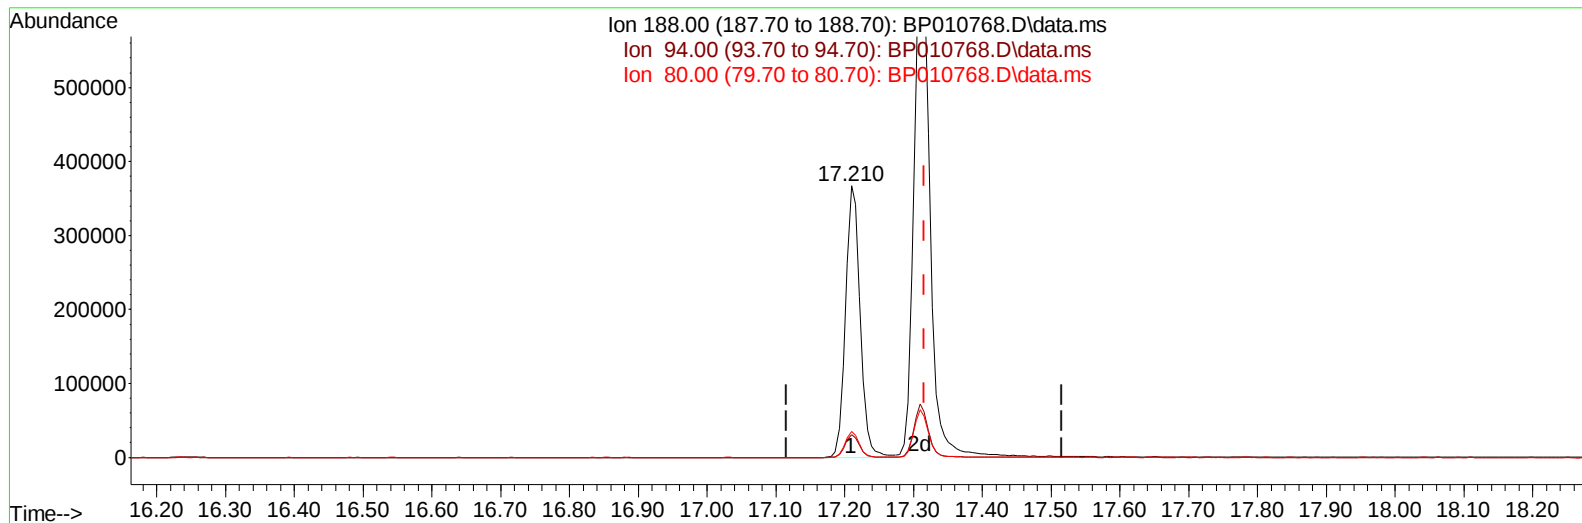

TIC: BP010768.D\data.ms

(73) Anthracene-d10 (S)

17.210min (-0.106) 22.05 ng/u1

response 545883

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.20	8.40
80.00	8.80	9.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010768.D
 Acq On : 20 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3358-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4S1

Manual IntegrationsAPPROVED

Quant Time: Jun 21 00:46:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

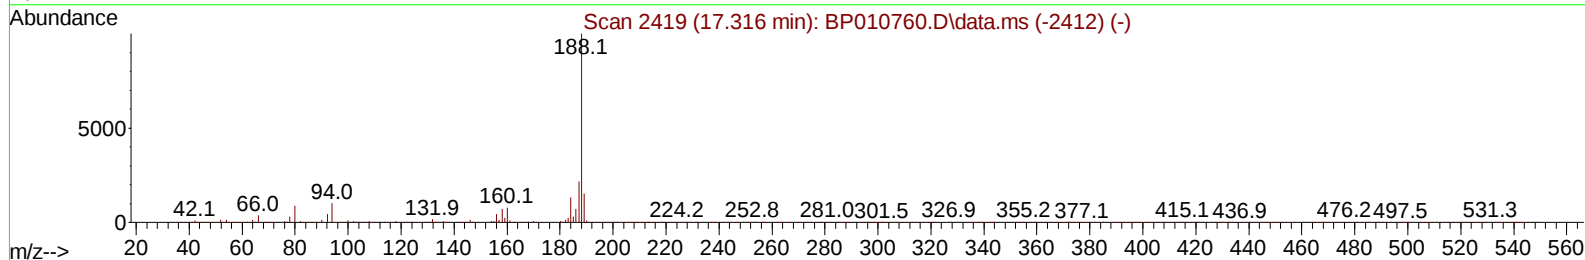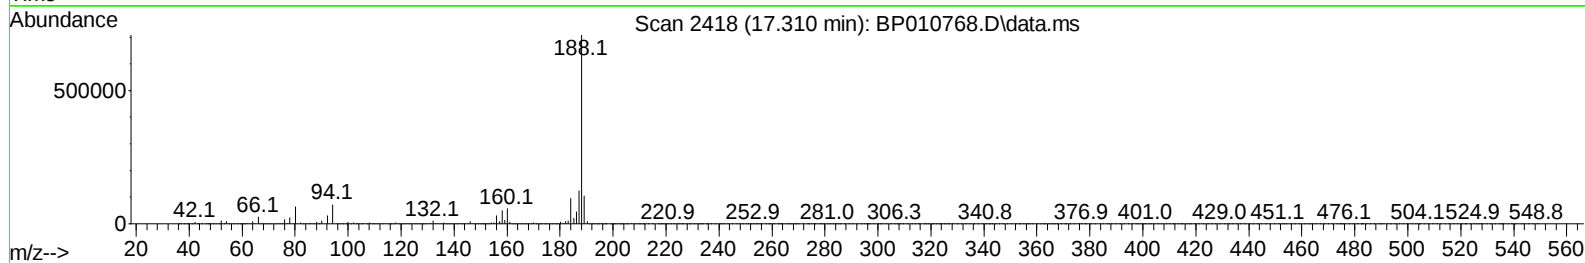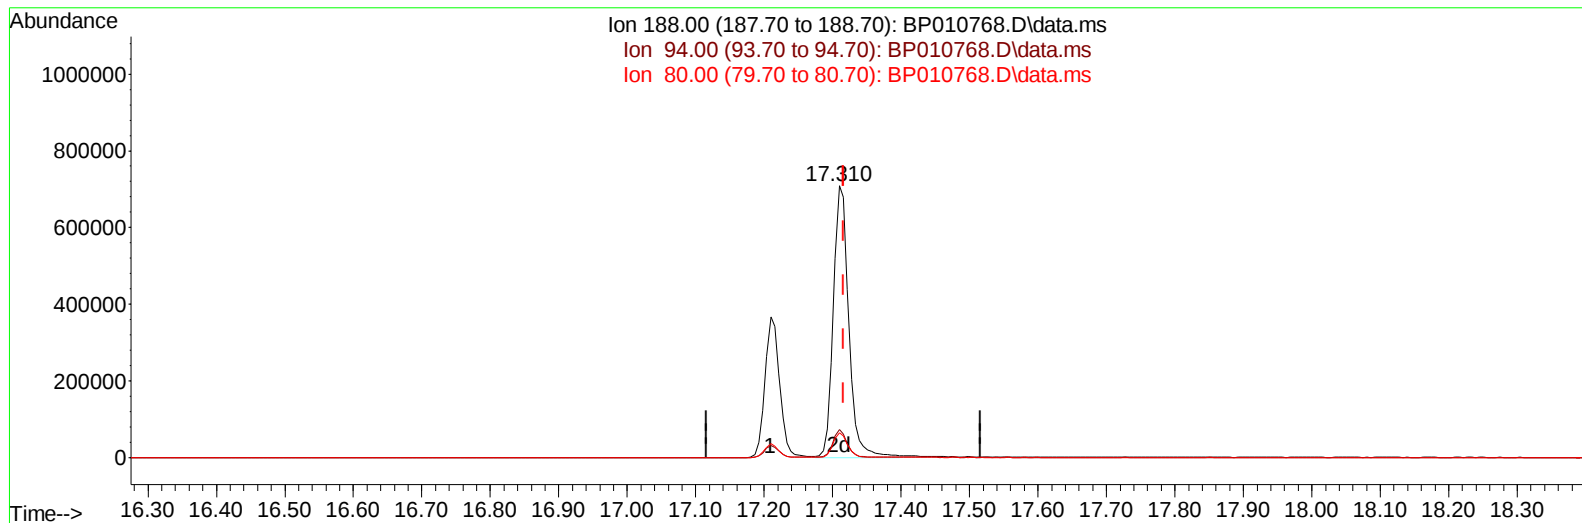

TIC: BP010768.D\data.ms

(73) Anthracene-d10 (S)

17.310min (-0.006) 44.78 ng/ul m

response 1108543

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.20	10.20#
80.00	8.80	9.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010768.D
 Acq On : 20 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3358-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4S1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 00:46:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	121828	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	457088	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	273708	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	545883	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	574232	20.000	ng/ul	0.00
88) Perylene-d12	23.698	264	658111	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	17569	6.198	ng/uL	0.00
4) Pyridine-d5	3.699	84	77123	10.462	ng/ul	0.00
7) Phenol-d5	7.004	99	66125	7.480	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.151	67	192818	35.824	ng/ul	0.00
11) 2-Chlorophenol-d4	7.351	132	215053	28.583	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	127908	17.907	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	127619m	37.604	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	132706	36.498	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	209587	31.110	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	270442	28.499	ng/ul	0.00
46) Dimethylphthalate-d6	13.869	166	768941	40.919	ng/ul	0.00
49) Acenaphthylene-d8	14.145	160	883729	38.832	ng/ul	0.00
54) 4-Nitrophenol-d4	14.733	143	14549m	5.241	ng/ul	0.05
60) Fluorene-d10	15.451	176	685549	41.042	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	101921	31.294	ng/ul	0.00
73) Anthracene-d10	17.310	188	1108543m	44.779	ng/ul	0.00
81) Pyrene-d10	19.551	212	1337771	46.863	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.545	264	1504988	45.925	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010768.D
Acq On : 20 Jun 2022 19:06
Operator : CG/JU
Sample : N3358-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4S1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 00:46:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 16:18:42 2022
Response via : Initial Calibration

