




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010769.D
 Acq On : 20 Jun 2022 19:40
 Operator : CG/JU
 Sample : N3358-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4R9

Manual IntegrationsAPPROVED

Quant Time: Jun 21 00:46:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

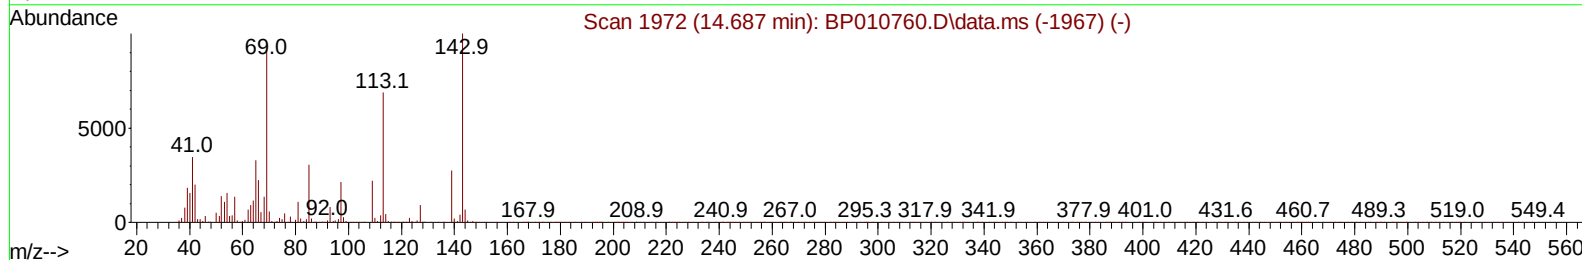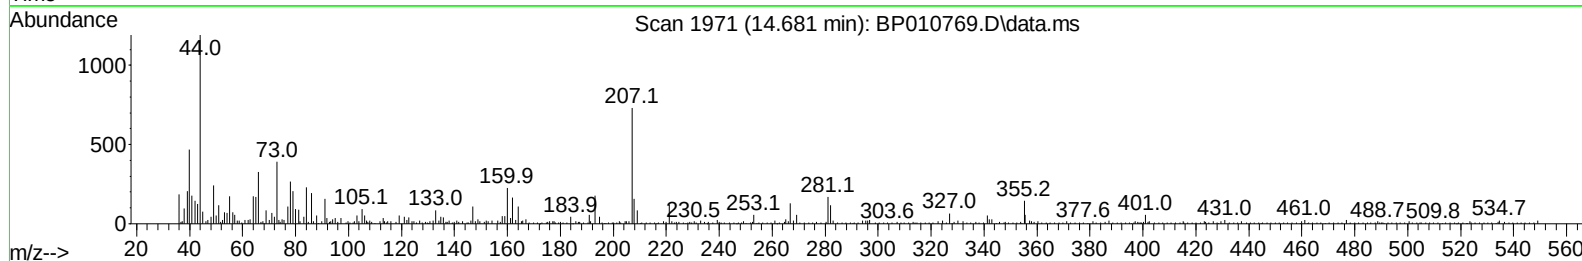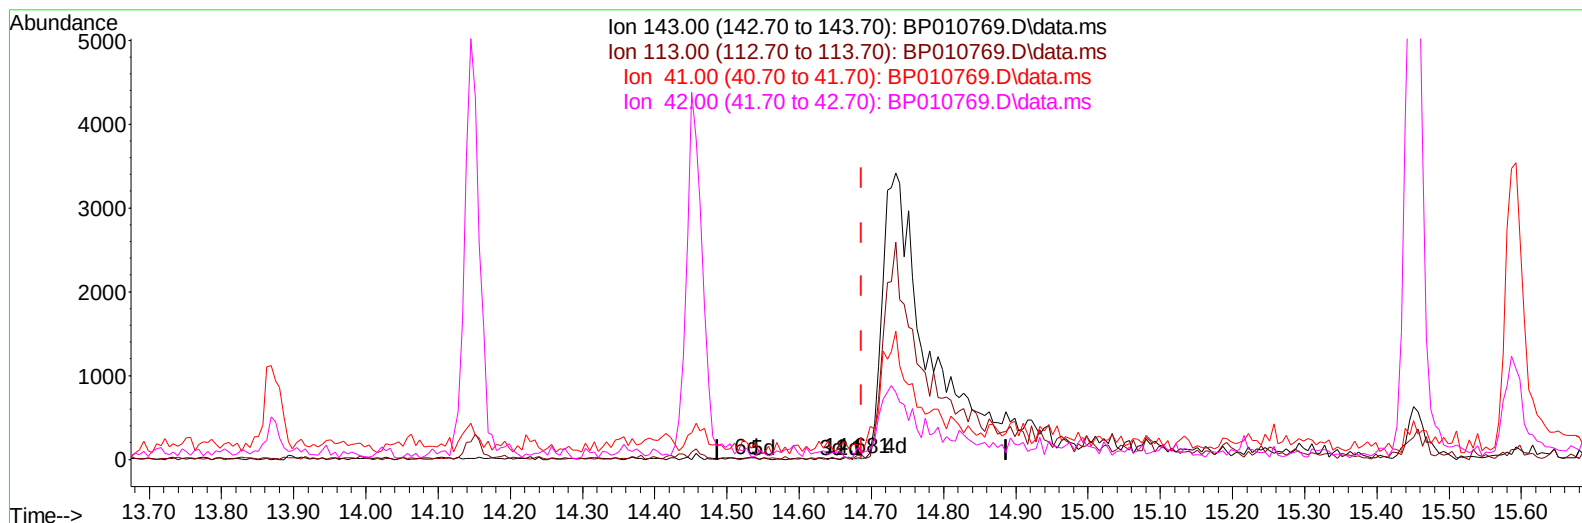

TIC: BP010769.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (-0.006) 0.00 ng/u1

response 11

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	294.44#
41.00	59.00	994.44#
42.00	41.10	800.00#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010769.D
 Acq On : 20 Jun 2022 19:40
 Operator : CG/JU
 Sample : N3358-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4R9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 00:46:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 16:18:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	107098	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	406735	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	255224	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	545656	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	604970	20.000	ng/ul	0.00
88) Perylene-d12	23.692	264	683419	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	13252	5.318	ng/uL	0.00
4) Pyridine-d5	3.722	84	18294	2.823	ng/ul	0.03
7) Phenol-d5	7.005	99	51579	6.637	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	144499	30.540	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	163848	24.772	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	97723	15.563	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	94881	31.419	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	97219	30.048	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	161000	26.857	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	142093	16.827	ng/ul	0.00
46) Dimethylphthalate-d6	13.869	166	631167	36.020	ng/ul	0.00
49) Acenaphthylene-d8	14.145	160	701478	33.056	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	13573m	5.244	ng/ul	0.05
60) Fluorene-d10	15.451	176	560780	36.003	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.586	200	88023	27.038	ng/ul	0.00
73) Anthracene-d10	17.310	188	981004	39.644	ng/ul	0.00
81) Pyrene-d10	19.551	212	1224966	40.731	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	1388192	40.792	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010769.D
Acq On : 20 Jun 2022 19:40
Operator : CG/JU
Sample : N3358-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4R9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 00:46:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 16:18:42 2022
Response via : Initial Calibration

