

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010765.D
 Acq On : 20 Jun 2022 17:25
 Operator : CG/JU
 Sample : PB145601BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	39	rVB	34809	45287	1.51%	0.160%
2	3.699	100	104	123	rBV	311949	579732	19.33%	2.050%
3	4.017	153	158	163	rVB	9834	16011	0.53%	0.057%
4	7.005	658	666	684	rBV	380661	692573	23.10%	2.449%
5	7.158	685	692	706	rVV	349151	579274	19.32%	2.048%
6	7.358	718	726	741	rBV	455654	764026	25.48%	2.702%
7	7.822	796	805	820	rBV	468292	774734	25.84%	2.740%
8	8.546	921	928	948	rBV	476806	869953	29.01%	3.076%
9	8.987	995	1003	1019	rBV	372730	678570	22.63%	2.400%
10	9.710	1118	1126	1137	rBV	299829	545845	18.20%	1.930%
11	10.257	1211	1219	1245	rBV	390794	840087	28.02%	2.971%
12	10.622	1273	1281	1293	rBV	589813	1026637	34.24%	3.630%
13	10.769	1299	1306	1331	rBV	376803	833209	27.79%	2.946%
14	12.234	1548	1555	1563	rBV3	6753	14767	0.49%	0.052%
15	13.881	1827	1835	1850	rBV	856086	1264070	42.16%	4.470%
16	13.981	1850	1852	1857	rVB6	2150	3101	0.10%	0.011%
17	14.157	1872	1882	1898	rBV	970423	1480027	49.36%	5.234%
18	14.463	1928	1934	1950	rBV	854687	1306638	43.58%	4.621%
19	14.710	1970	1976	2001	rBV3	102576	425419	14.19%	1.504%
20	15.463	2097	2104	2119	rBV	1264964	1954701	65.19%	6.912%
21	15.598	2121	2127	2142	rVV	277935	483544	16.13%	1.710%
22	15.704	2142	2145	2150	rVB2	16714	26102	0.87%	0.092%
23	16.251	2234	2238	2243	rVB6	4829	6715	0.22%	0.024%
24	16.716	2312	2317	2324	rBV6	3139	7918	0.26%	0.028%
25	16.904	2343	2349	2353	rBV8	3319	5150	0.17%	0.018%
26	17.222	2397	2403	2414	rBV	1044249	1500491	50.04%	5.306%
27	17.322	2414	2420	2433	rVV2	1353435	2065077	68.87%	7.303%
28	17.863	2508	2512	2516	rBV7	4933	8964	0.30%	0.032%
29	19.139	2726	2729	2734	rVB4	17975	22346	0.75%	0.079%
30	19.210	2738	2741	2745	rBV2	16341	21957	0.73%	0.078%
31	19.563	2795	2801	2807	rBV	1864669	2536077	84.58%	8.968%
32	19.610	2807	2809	2817	rVB	66850	111799	3.73%	0.395%
33	21.316	3094	3099	3107	rBV	1336696	1854729	61.85%	6.559%
34	23.557	3473	3480	3496	rBV2	1413391	2998583	100.00%	10.604%
35	23.716	3500	3507	3517	rVB2	912679	1934304	64.51%	6.840%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010765.D
Acq On : 20 Jun 2022 17:25
Operator : CG/JU
Sample : PB145601BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK601

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Title : SVOA CALIBRATION




Sum of corrected areas: 28278417

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010765.D
Acq On : 20 Jun 2022 17:25
Operator : CG/JU
Sample : PB145601BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK601

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

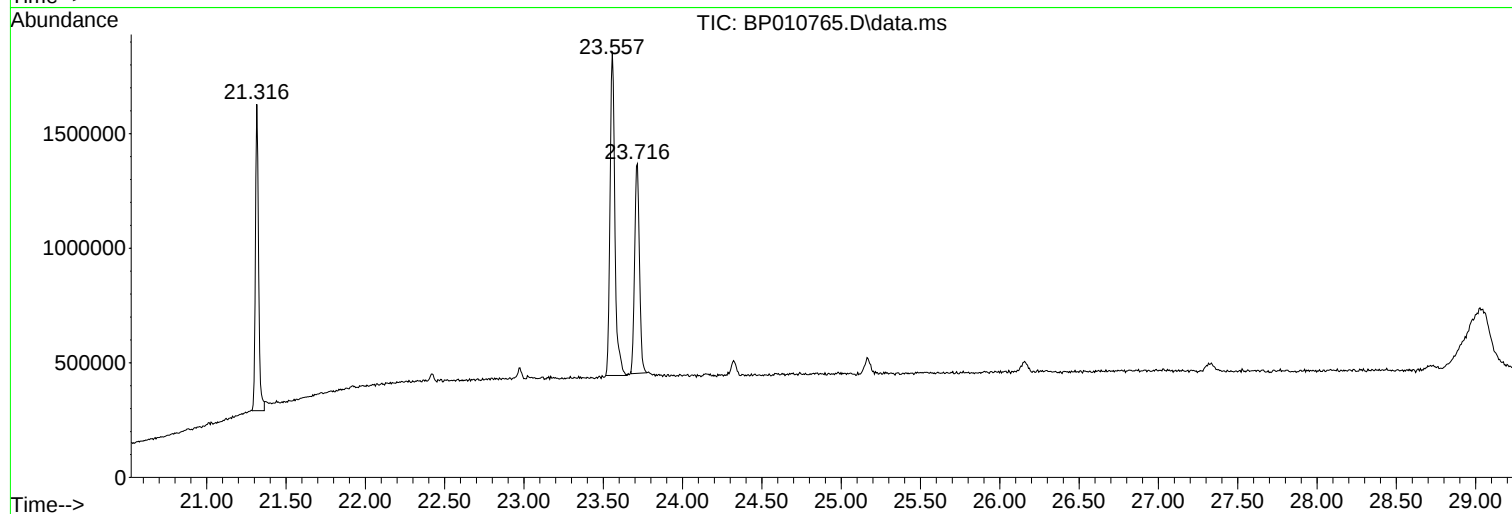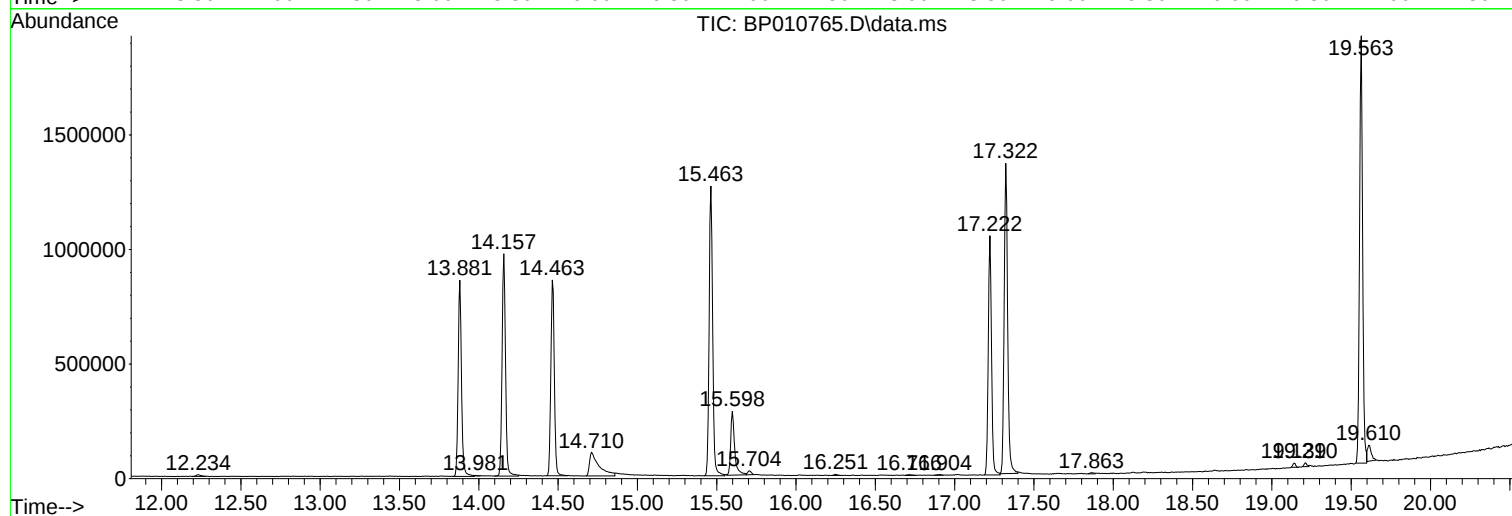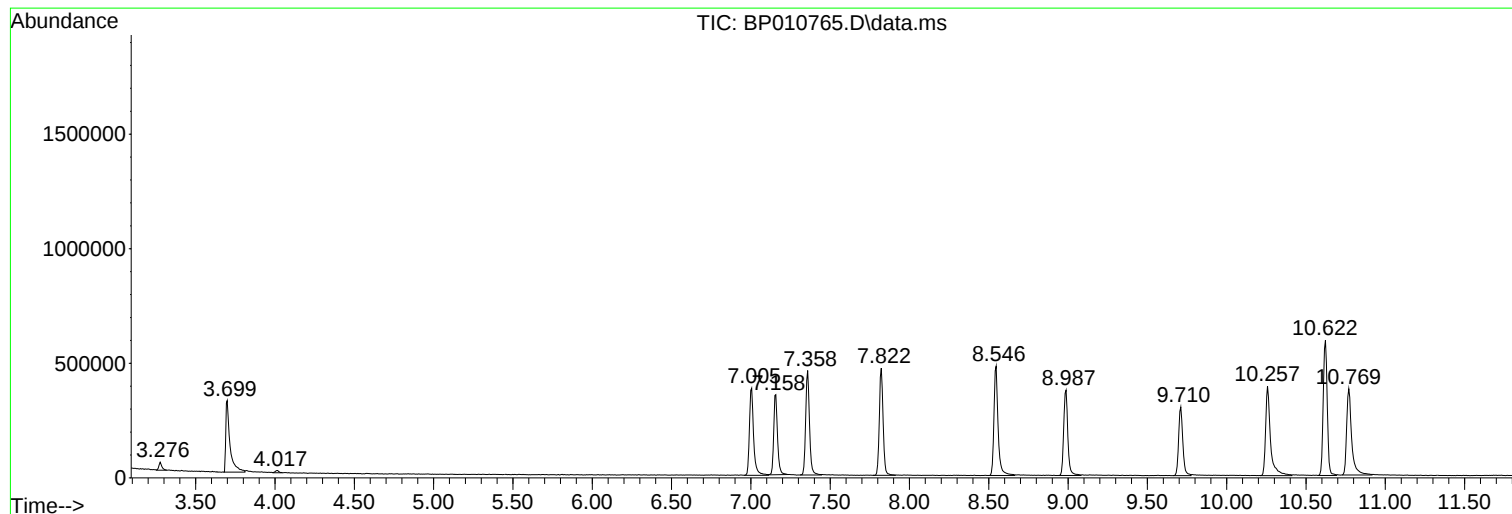

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010765.D
Acq On : 20 Jun 2022 17:25
Operator : CG/JU
Sample : PB145601BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK601

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010765.D
Acq On : 20 Jun 2022 17:25
Operator : CG/JU
Sample : PB145601BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK601

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc