

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010768.D
 Acq On : 20 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3358-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	39	rVB	32574	39296	1.05%	0.132%
2	3.699	101	104	121	rBV	107356	214897	5.77%	0.720%
3	3.916	137	141	145	rVB2	13036	20068	0.54%	0.067%
4	4.010	153	157	162	rVB	10879	13587	0.36%	0.046%
5	4.569	249	252	257	rVB6	2892	4972	0.13%	0.017%
6	4.804	287	292	295	rBV6	2805	4758	0.13%	0.016%
7	4.928	306	313	319	rBV3	6991	13406	0.36%	0.045%
8	7.004	655	666	684	rBV	93009	193794	5.20%	0.650%
9	7.151	684	691	709	rBV	426271	715072	19.20%	2.397%
10	7.351	718	725	737	rBV	420379	721919	19.38%	2.420%
11	7.816	792	804	814	rBV	420251	690680	18.54%	2.316%
12	8.540	919	927	943	rBV	290833	546243	14.66%	1.831%
13	8.981	994	1002	1026	rBV	469805	851055	22.85%	2.853%
14	9.698	1117	1124	1142	rBV	368095	669331	17.97%	2.244%
15	10.251	1206	1218	1240	rBV	436230	951132	25.53%	3.189%
16	10.610	1271	1279	1296	rBV	523927	920272	24.71%	3.085%
17	10.763	1296	1305	1323	rBV	391834	858979	23.06%	2.880%
18	11.910	1493	1500	1503	rBV8	1660	4134	0.11%	0.014%
19	11.986	1506	1513	1518	rVV8	2781	5328	0.14%	0.018%
20	12.222	1547	1553	1559	rBV3	8038	16678	0.45%	0.056%
21	13.286	1729	1734	1740	rVB10	2963	5421	0.15%	0.018%
22	13.433	1755	1759	1766	rBV10	3174	4717	0.13%	0.016%
23	13.869	1827	1833	1855	rBV	1070417	1579797	42.41%	5.297%
24	14.145	1872	1880	1897	rBV	1205726	1887301	50.67%	6.328%
25	14.457	1925	1933	1945	rBV	778984	1156717	31.05%	3.878%
26	14.739	1973	1981	1990	rBV4	19601	68057	1.83%	0.228%
27	15.216	2057	2062	2068	rBV	27910	42257	1.13%	0.142%
28	15.310	2077	2078	2084	rVB5	2985	3965	0.11%	0.013%
29	15.451	2096	2102	2120	rBV	1648921	2500548	67.13%	8.384%
30	15.586	2120	2125	2138	rVV	345491	623869	16.75%	2.092%
31	15.698	2140	2144	2153	rVB2	23530	42322	1.14%	0.142%
32	16.239	2233	2236	2242	rVB7	5986	9344	0.25%	0.031%
33	16.892	2342	2347	2352	rVB9	4348	5955	0.16%	0.020%
34	16.980	2359	2362	2364	rBV4	2863	3935	0.11%	0.013%
35	17.210	2394	2401	2412	rBV	860110	1298914	34.87%	4.355%
36	17.310	2412	2418	2433	rVV	1743658	2720149	73.03%	9.120%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
 Data File : BP010768.D
 Acq On : 20 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3358-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
 Title : SVOA CALIBRATION

37	18.104	2550	2553	2559	rBV8	11034	18567	0.50%	0.062%
38	19.127	2724	2727	2731	rBV4	24379	29115	0.78%	0.098%
39	19.204	2736	2740	2744	rVV2	20206	29986	0.81%	0.101%
40	19.551	2793	2799	2811	rBV	2566262	3371393	90.51%	11.303%
41	21.310	3093	3098	3107	rBV	1056346	1518246	40.76%	5.090%
42	23.545	3471	3478	3489	rBV	1861855	3724878	100.00%	12.489%
43	23.698	3498	3504	3518	rVB2	787897	1725094	46.31%	5.784%




Sum of corrected areas: 29826148

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010768.D
Acq On : 20 Jun 2022 19:06
Operator : CG/JU
Sample : N3358-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4S1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

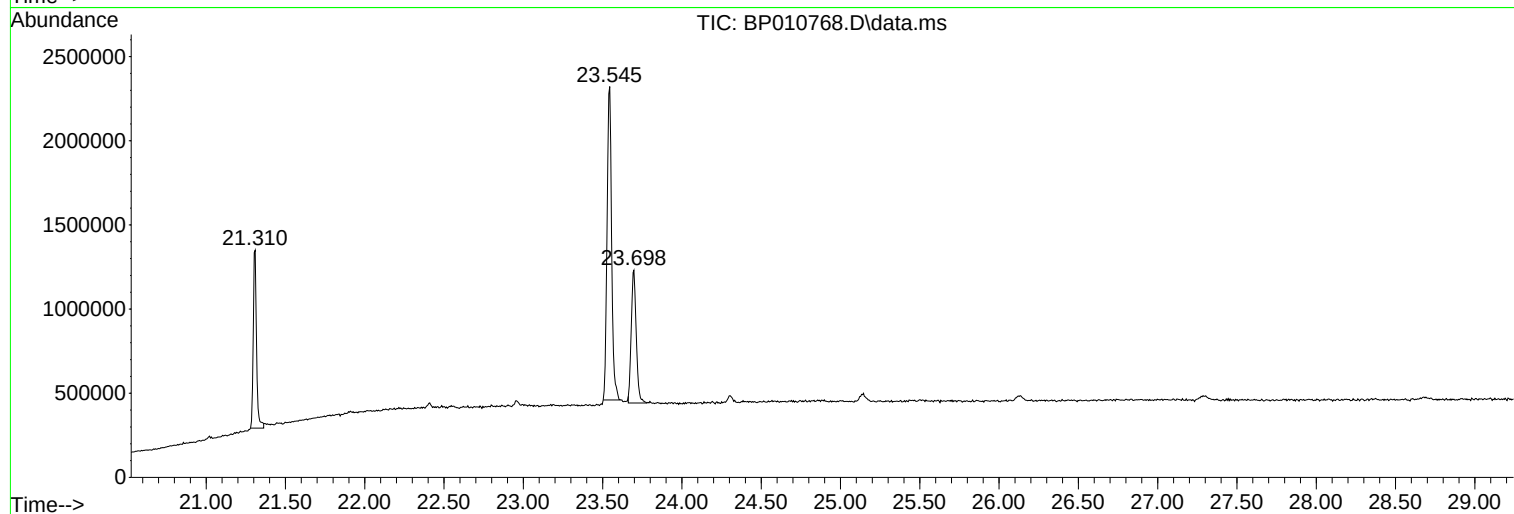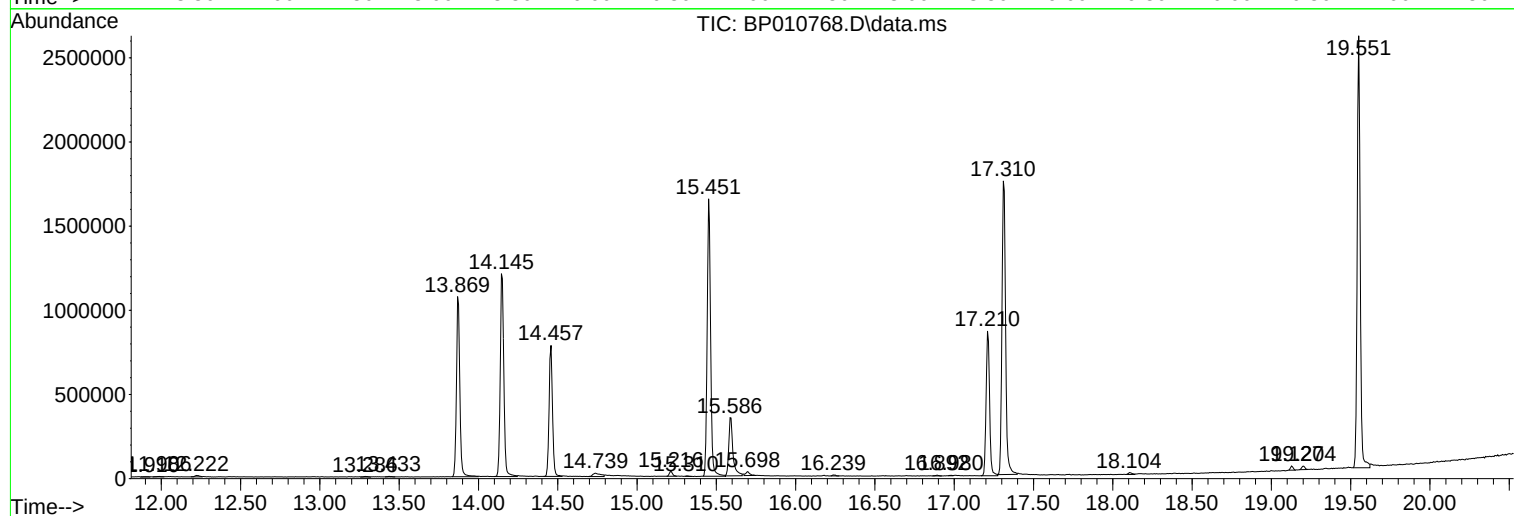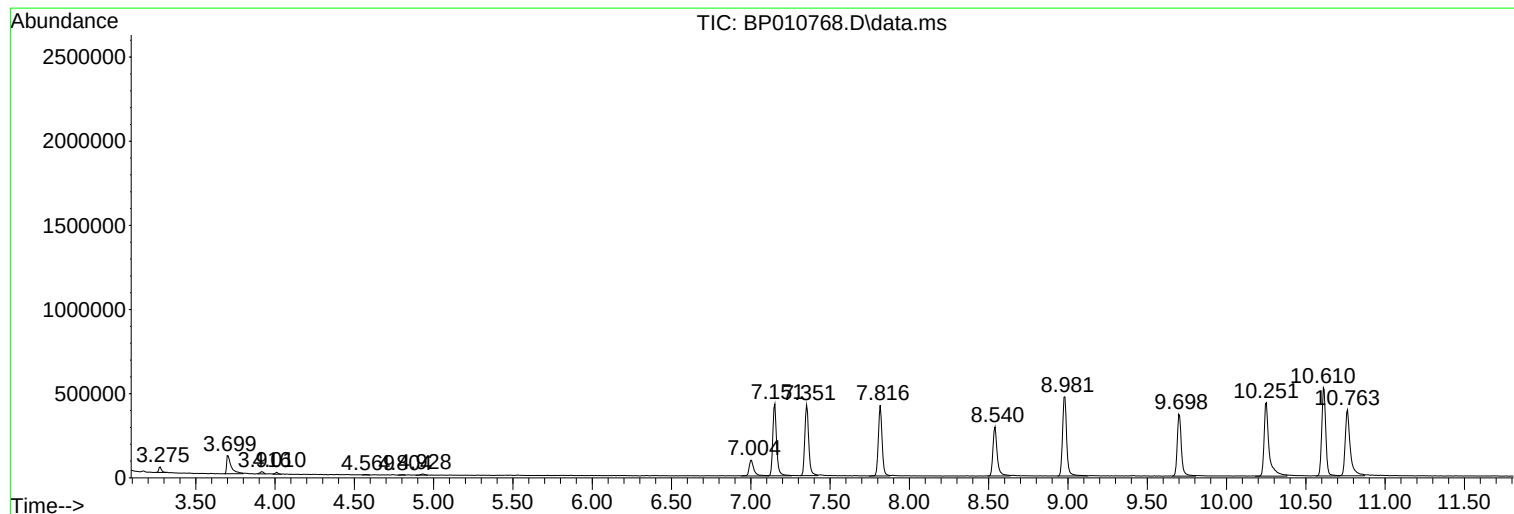

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010768.D
Acq On : 20 Jun 2022 19:06
Operator : CG/JU
Sample : N3358-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4S1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062022\
Data File : BP010768.D
Acq On : 20 Jun 2022 19:06
Operator : CG/JU
Sample : N3358-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4S1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc