
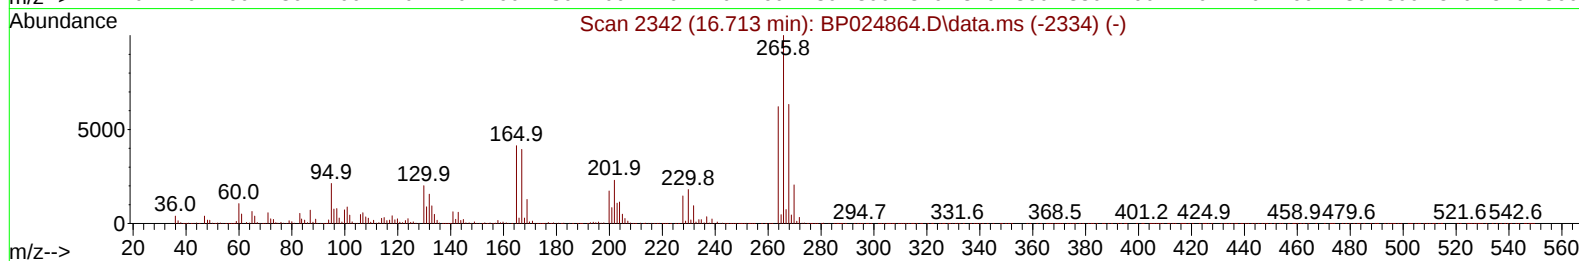
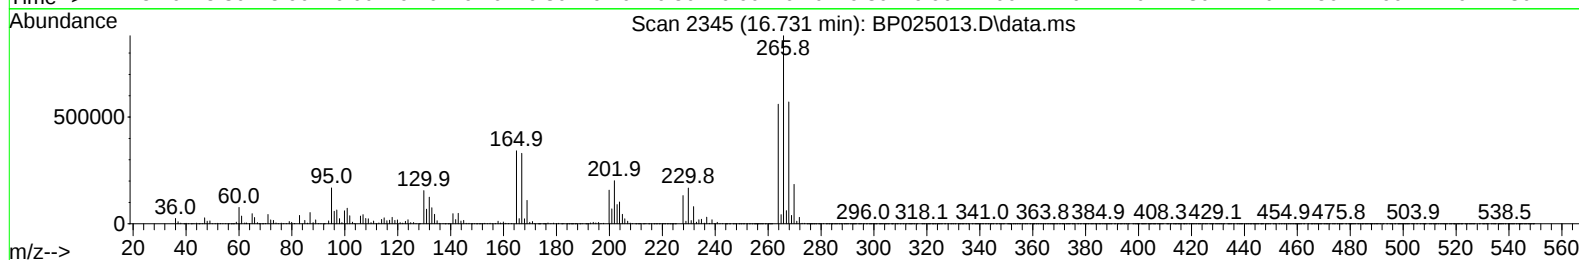


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062025\
Data File : BP025013.D
Acq On : 20 Jun 2025 11:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 12:54:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

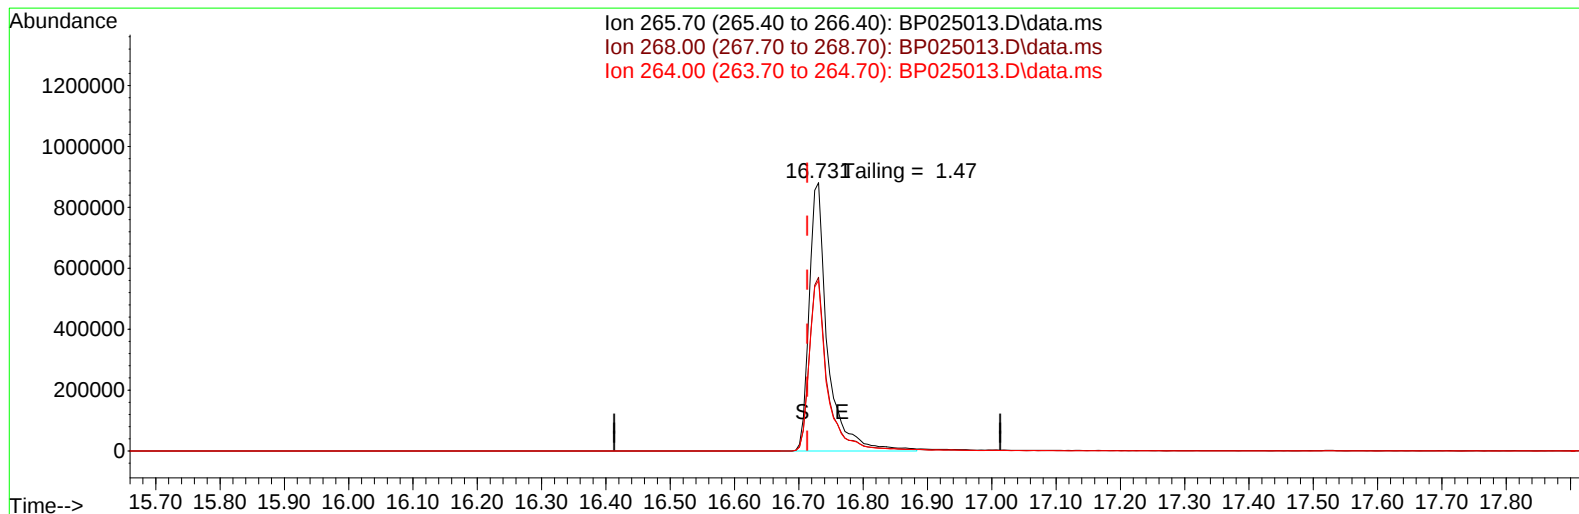

TIC: BP025013.D\data.ms

(70) Pentachlorophenol (C)




16.731min (+ 0.018) 3960724.34 ng

response 1766478

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.75
264.00	62.10	63.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062025\
Data File : BP025013.D
Acq On : 20 Jun 2025 11:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 12:54:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

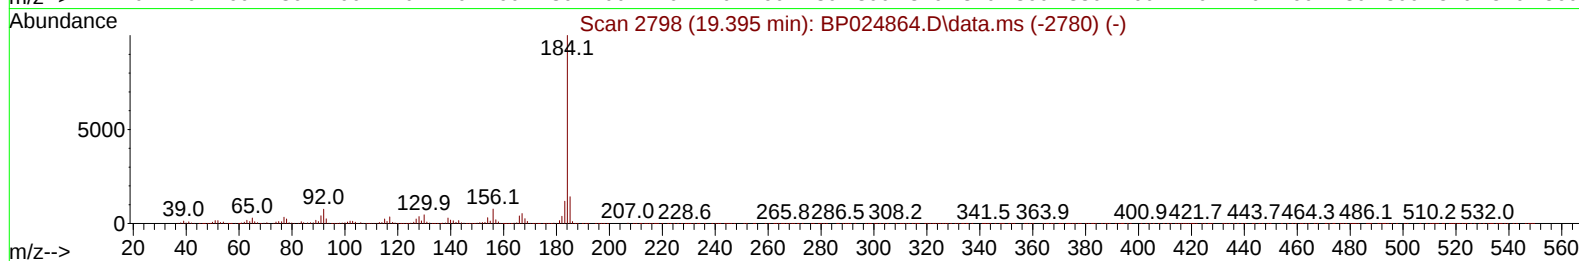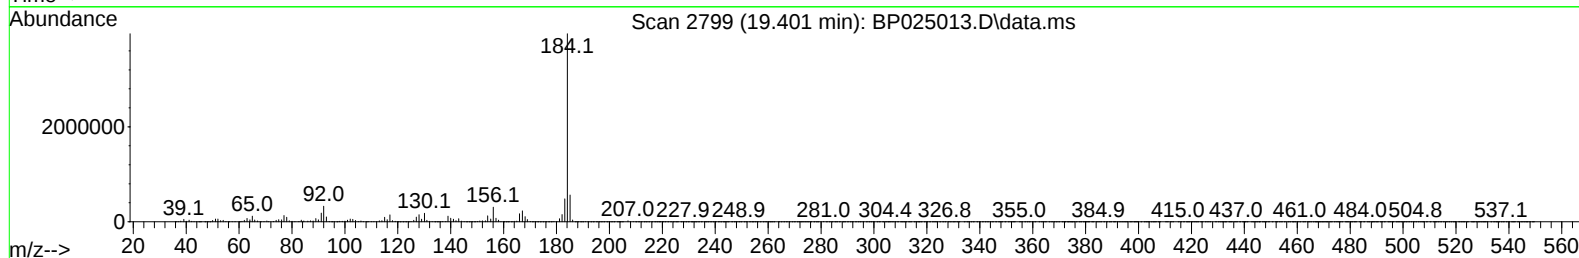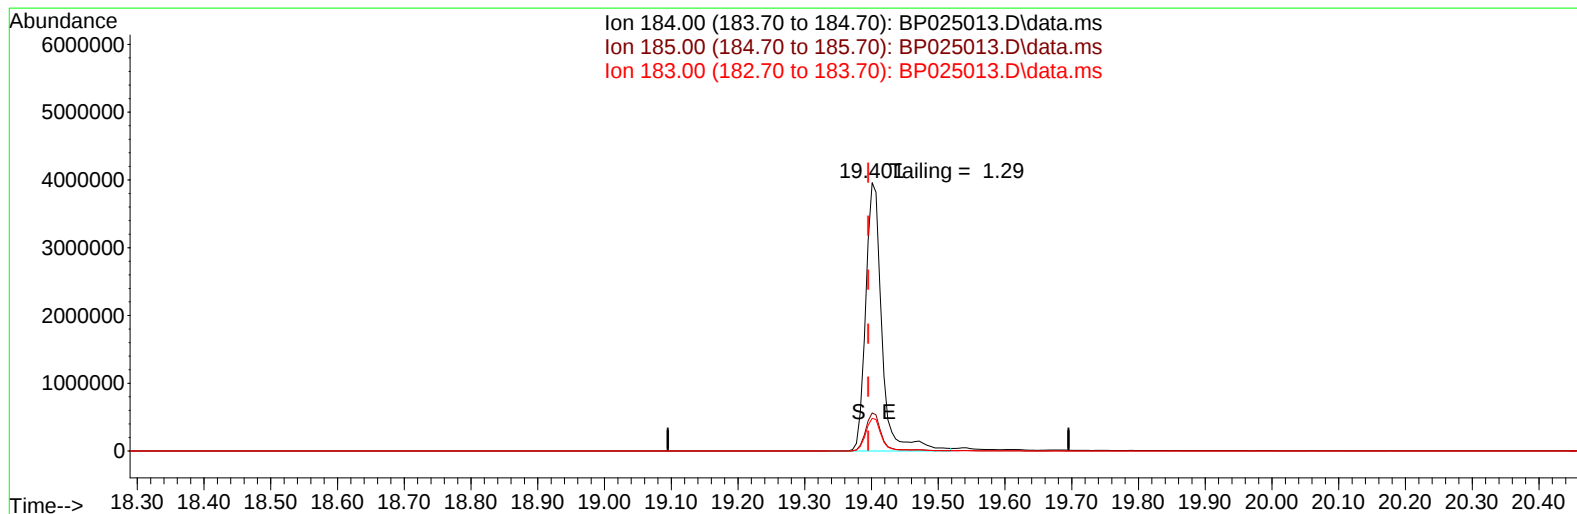

TIC: BP025013.D\data.ms

(77) Benzidine**19.401min (+ 0.006) 1030641.18 ng****response 6416011**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.18
183.00	11.90	12.20
0.00	0.00	0.00