
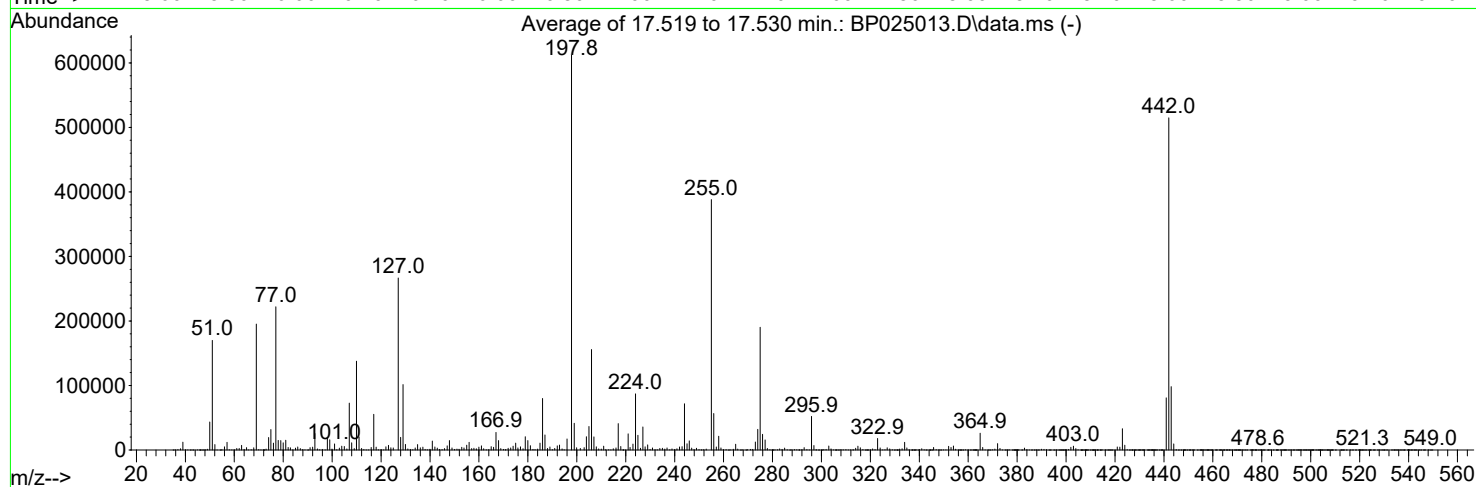


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062025\
Data File : BP025013.D
Acq On : 20 Jun 2025 11:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 06 16:20:27 2025

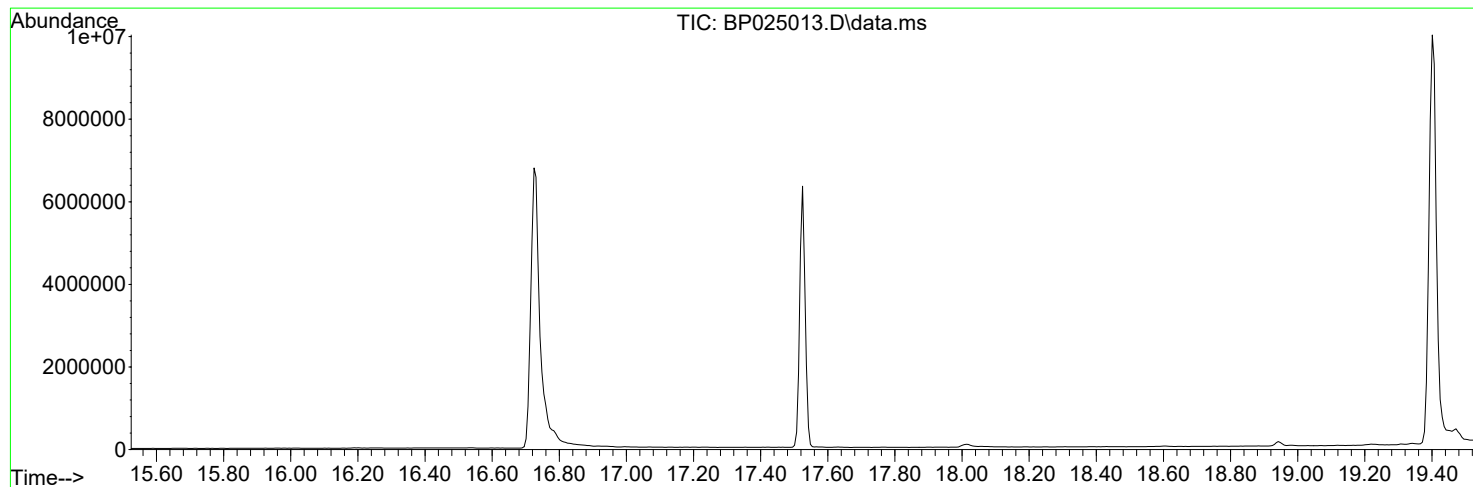

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3363	PASS
69	69	100	100	100.0	195122	PASS
70	69	0.00	2	0.4	873	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	611957	PASS
199	198	5	9	6.8	41533	PASS
365	198	1	100	4.3	26067	PASS
441	443	0.01	150	82.3	80743	PASS
442	442	100	100	100.0	514816	PASS
443	442	15	24	19.1	98128	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/20/2025	BNA_P	<u>BP025002.D</u>
Compound Name	Response	Retention Time
DDT	2098688	20.677
DDD	61093	20.224
DDE	5431	19.695
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
66524	2165212	3.07

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062025\
Data File : BP025013.D
Acq On : 20 Jun 2025 11:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 20 12:54:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

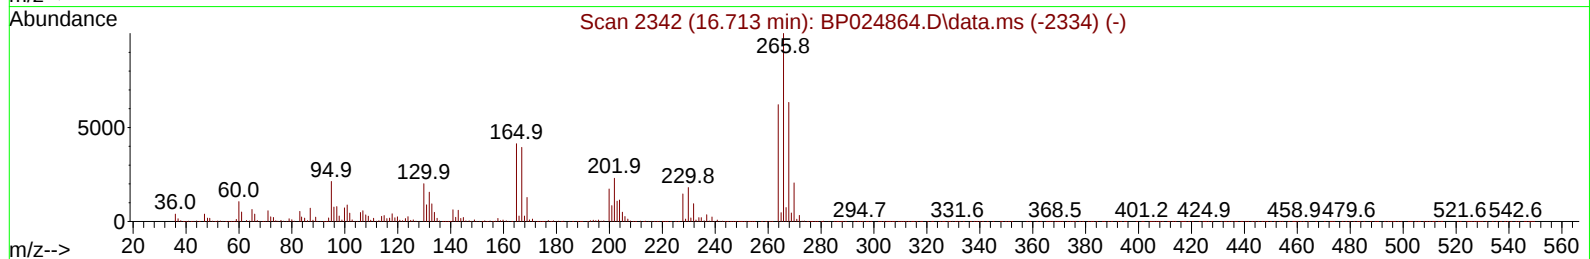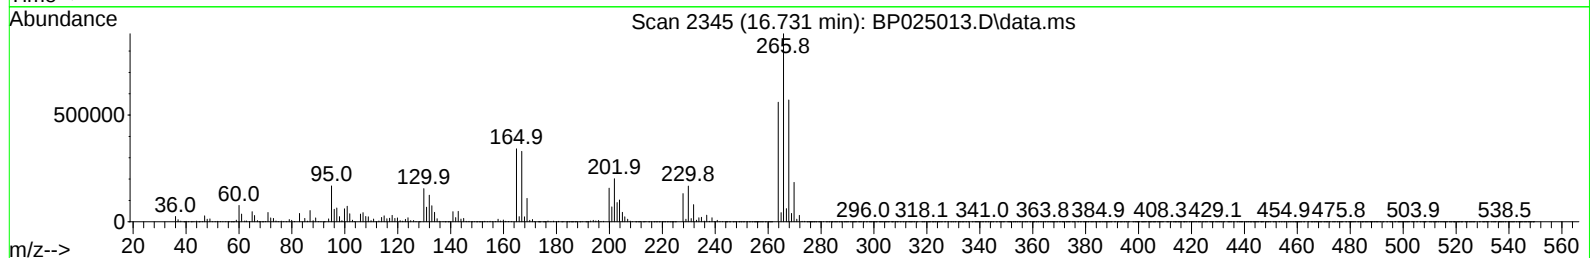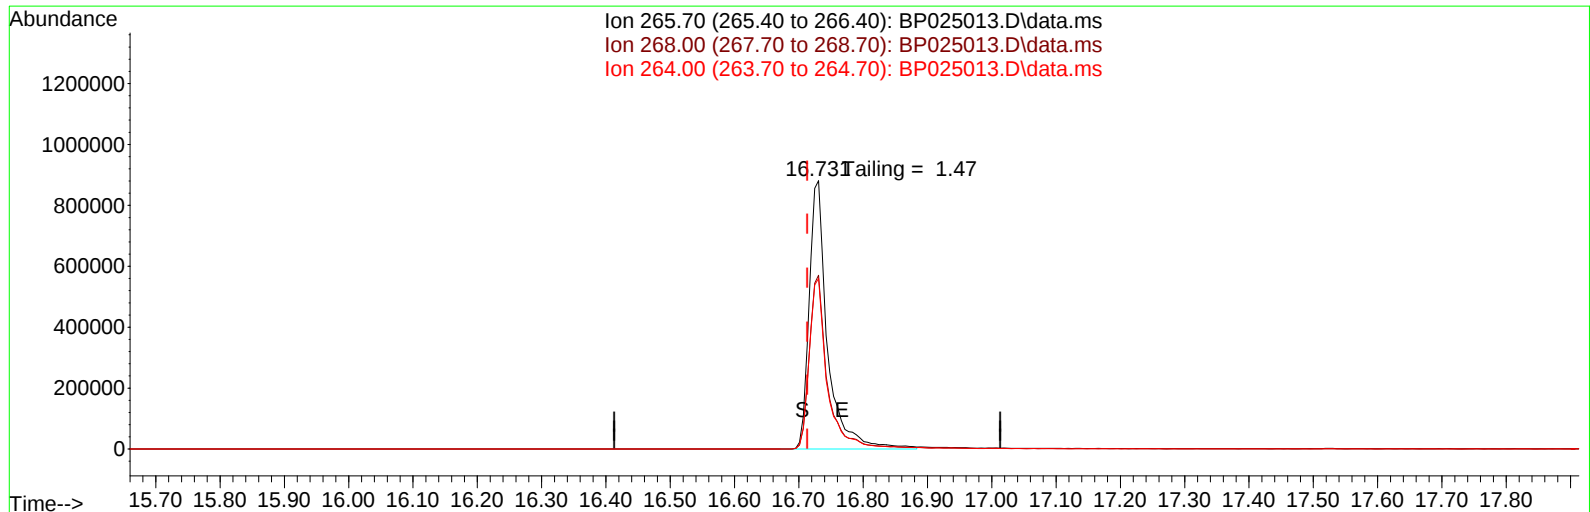

TIC: BP025013.D\data.ms

(70) Pentachlorophenol (C)

16.731min (+ 0.018) 3960724.34 ng




response 1766478

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.75
264.00	62.10	63.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062025\
Data File : BP025013.D
Acq On : 20 Jun 2025 11:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 20 12:54:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

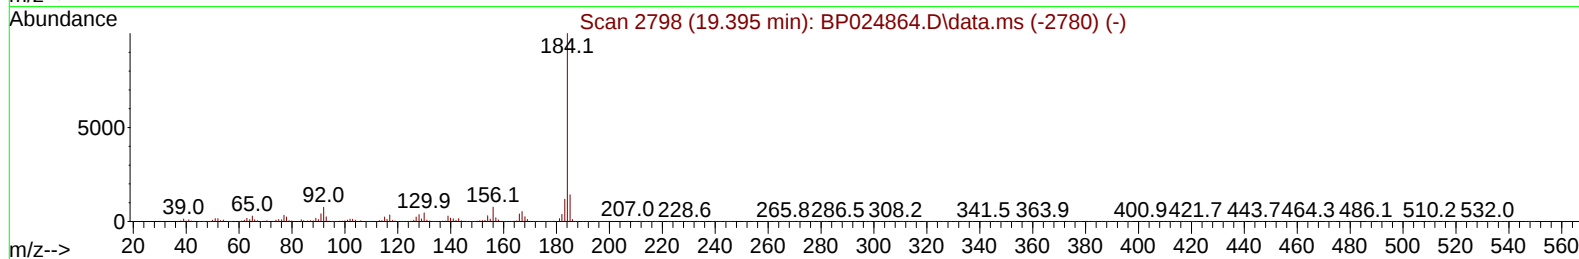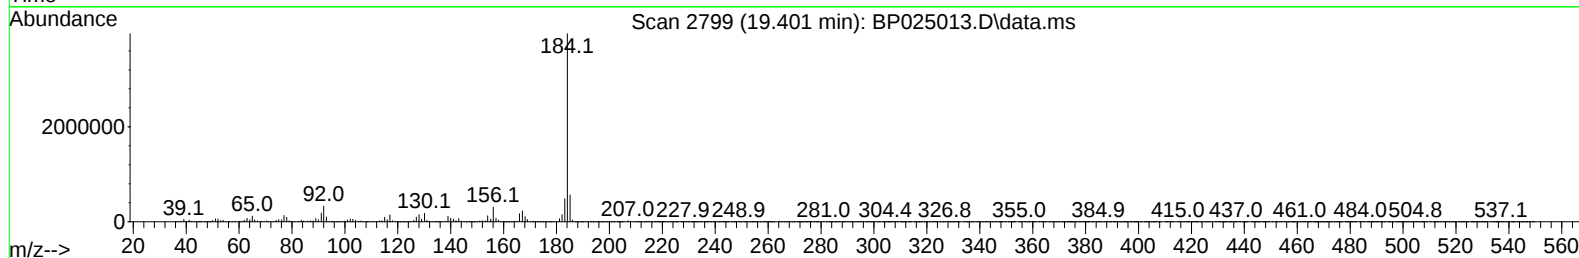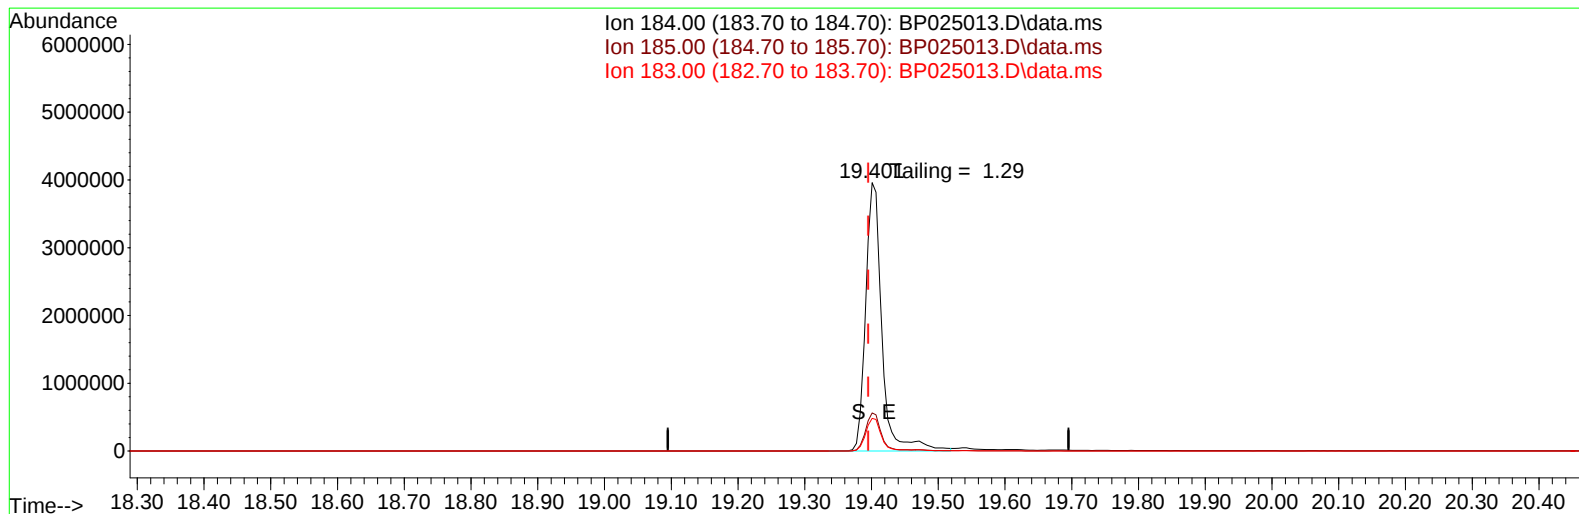

TIC: BP025013.D\data.ms

(77) Benzidine

19.401min (+ 0.006) 1030641.18 ng

response 6416011

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.18
183.00	11.90	12.20
0.00	0.00	0.00