
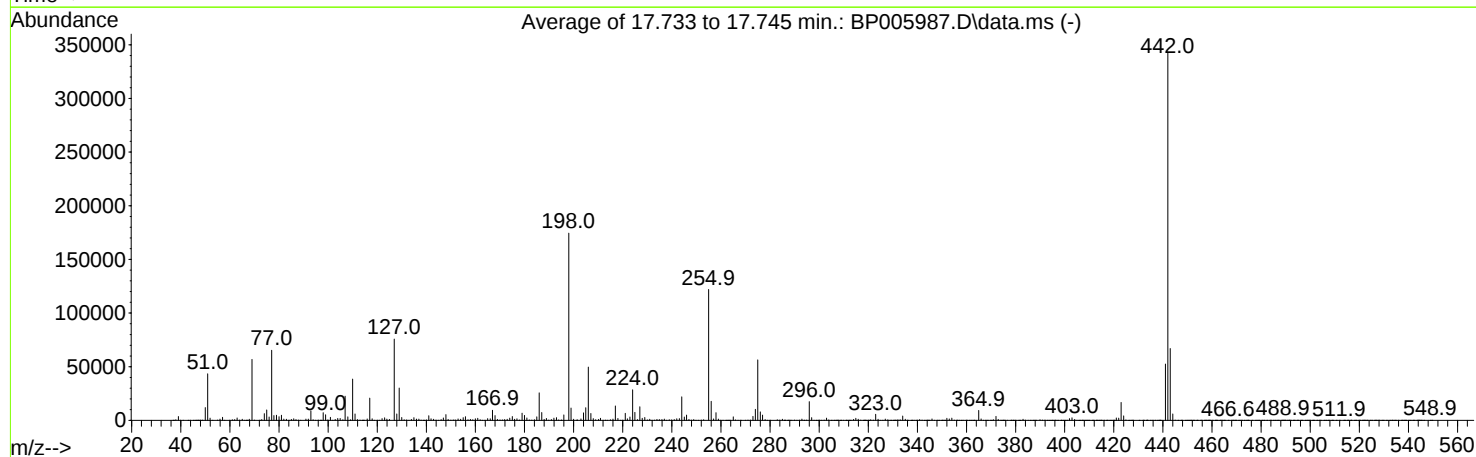


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062121\
 Data File : BP005987.D
 Acq On : 21 Jun 2021 10:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 23 11:35:30 2021

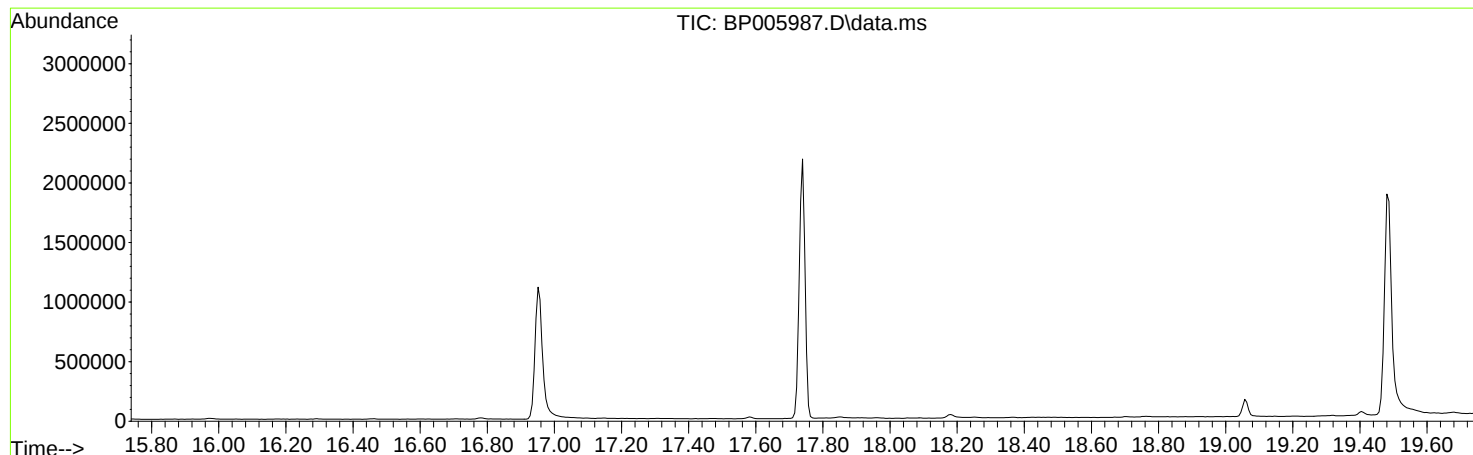

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	43343	PASS
68	69	0.00	2	2.0	1117	PASS
69	198	0.00	100	32.5	56779	PASS
70	69	0.00	2	0.5	273	PASS
127	198	10	80	43.4	75791	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	174520	PASS
199	198	5	9	6.6	11530	PASS
275	198	10	60	32.3	56357	PASS
365	198	1	100	5.3	9195	PASS
441	198	0.01	100	30.1	52459	PASS
442	442	100	100	100.0	342819	PASS
443	442	15	24	19.5	66965	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/21/2021	BNA_P	<u>BP005987.D</u>
Compound Name	Response	Retention Time
DDT	736878	20.67
DDD	22453	20.25
DDE	2944	20.25
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25397	762275	3.33

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062121\
 Data File : BP005987.D
 Acq On : 21 Jun 2021 10:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 21 11:35:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 11:35:30 2021
 Response via : Initial Calibration

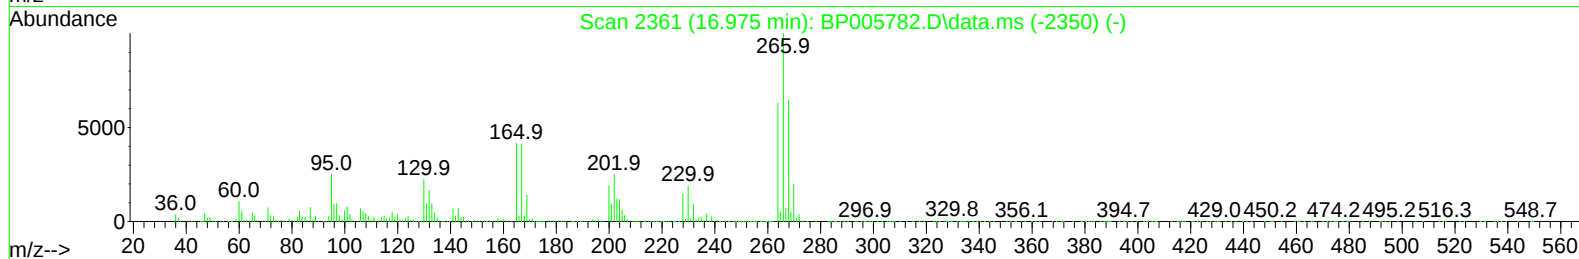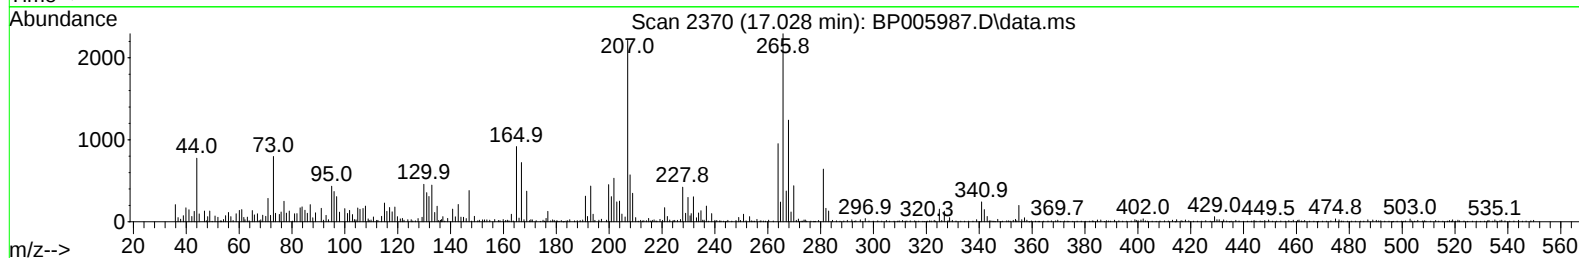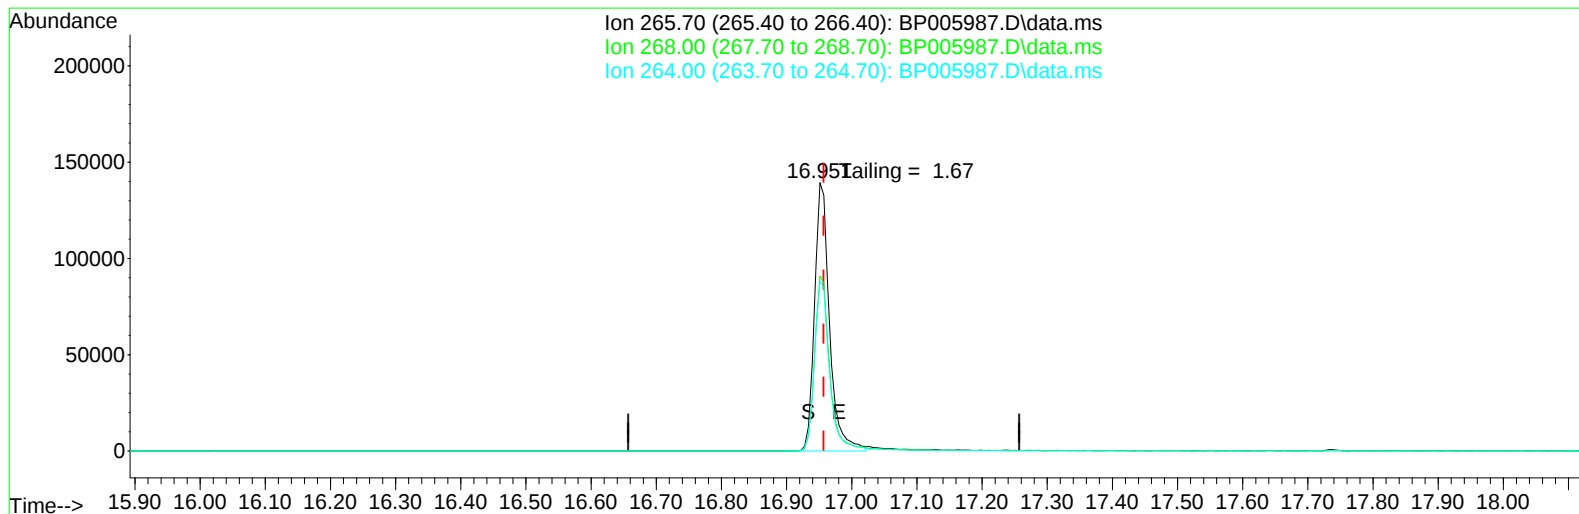

TIC: BP005987.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.006) 765140.09 ng




response 229086

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.18
264.00	62.90	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062121\
 Data File : BP005987.D
 Acq On : 21 Jun 2021 10:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 21 11:35:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 11:35:30 2021
 Response via : Initial Calibration

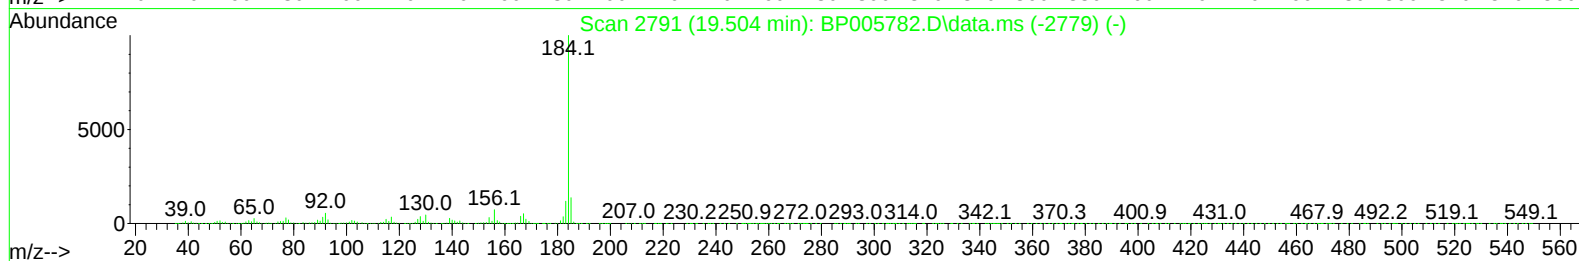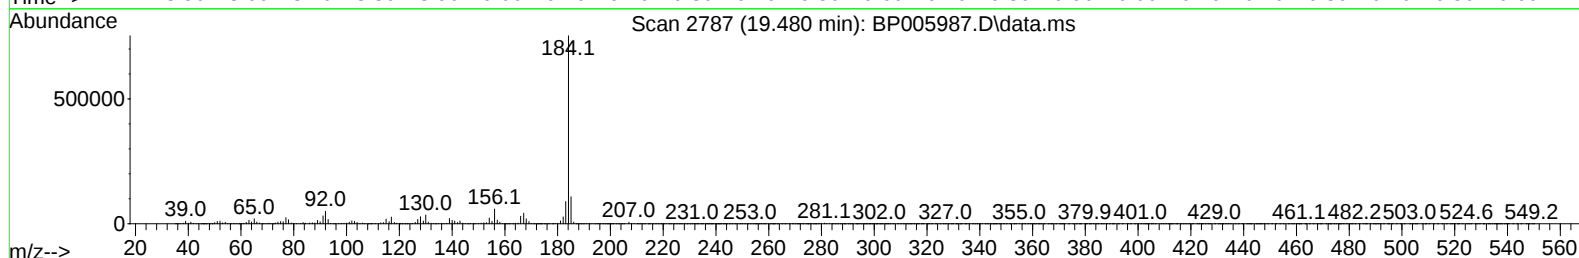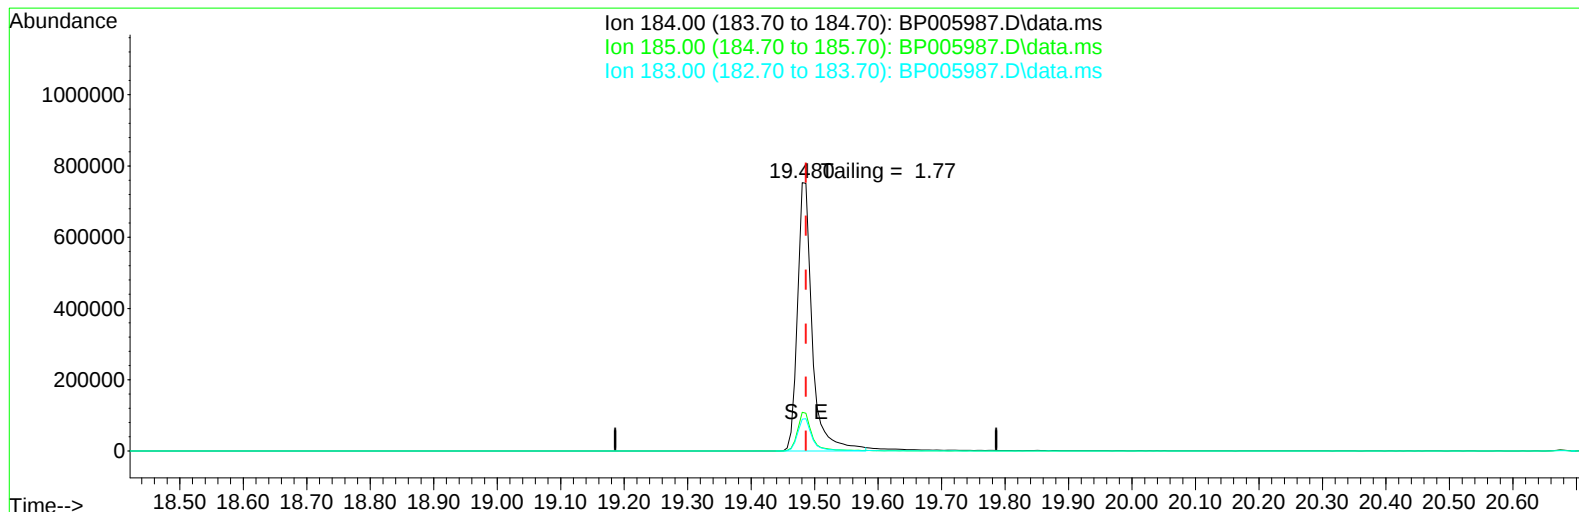

TIC: BP005987.D\data.ms

(77) Benzidine

19.480min (-0.006) 314246.60 ng

response 1255458

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.42
183.00	11.90	11.86
0.00	0.00	0.00