


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062220\
 Data File : BP002473.D
 Acq On : 22 Jun 2020 09:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

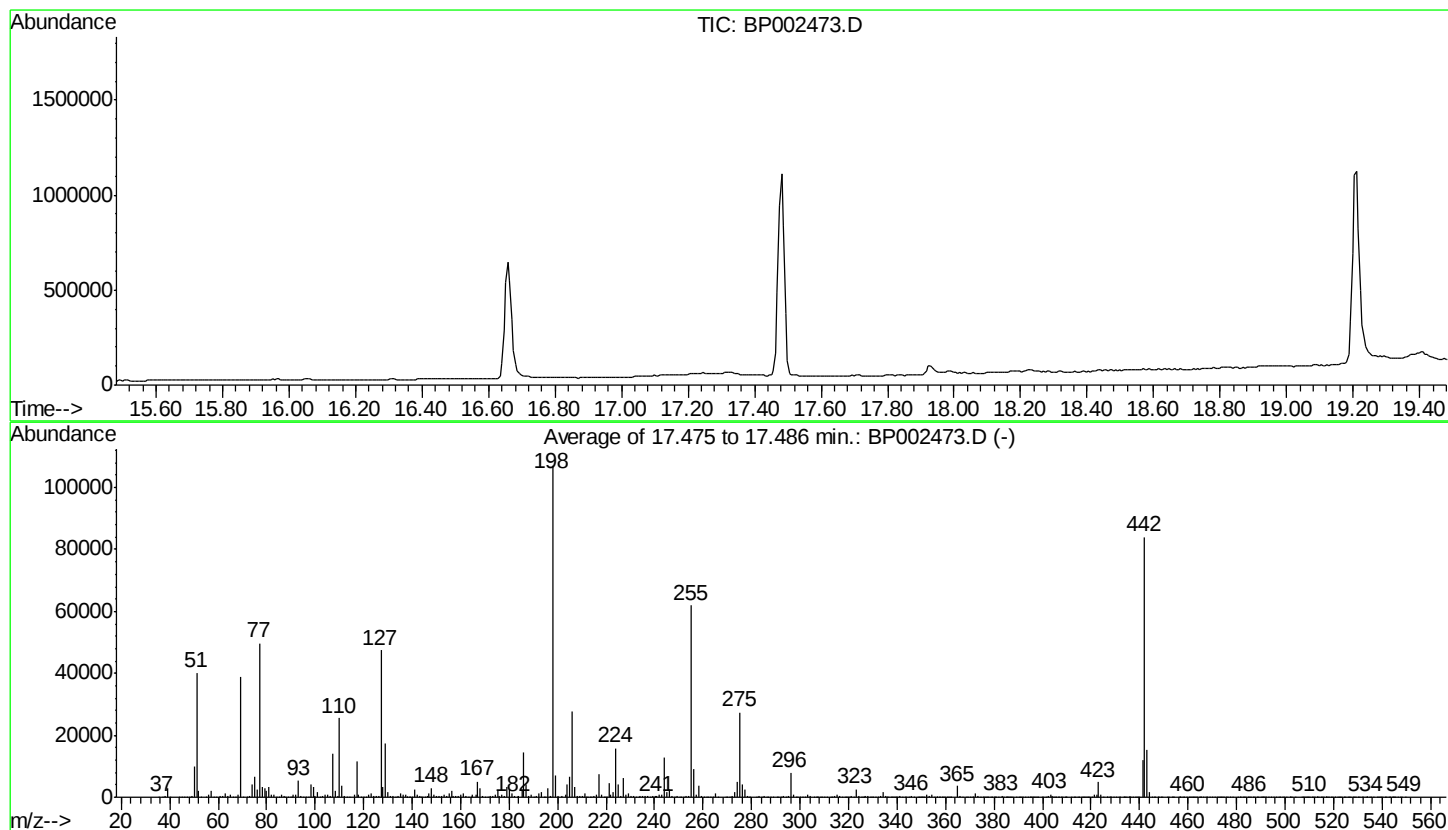

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	40245	PASS
68	69	0.00	2	1.6	639	PASS
69	198	0.00	100	36.4	38986	PASS
70	69	0.00	2	0.4	172	PASS
127	198	10	80	44.3	47440	PASS
197	198	0.00	2	0.4	467	PASS
198	198	100	100	100.0	107083	PASS
199	198	5	9	6.7	7153	PASS
275	198	10	60	25.5	27353	PASS
365	198	1	100	3.5	3698	PASS
441	198	0.01	100	11.3	12135	PASS
442	198	50	100	78.4	83928	PASS
443	442	15	24	18.3	15346	PASS