
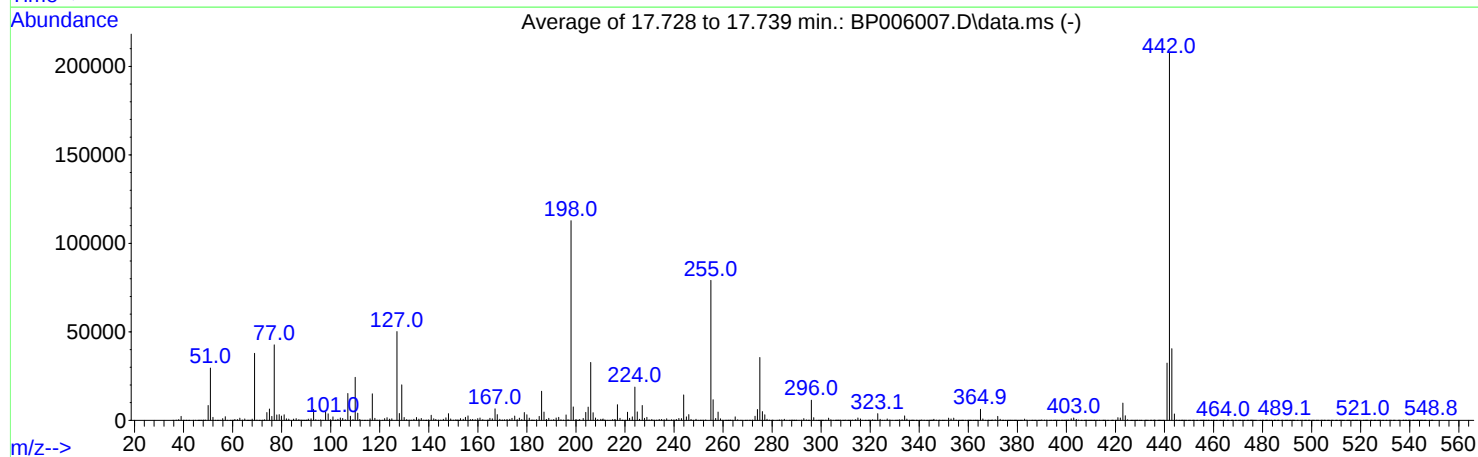


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062221\
 Data File : BP006007.D
 Acq On : 22 Jun 2021 15:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 22 17:52:38 2021

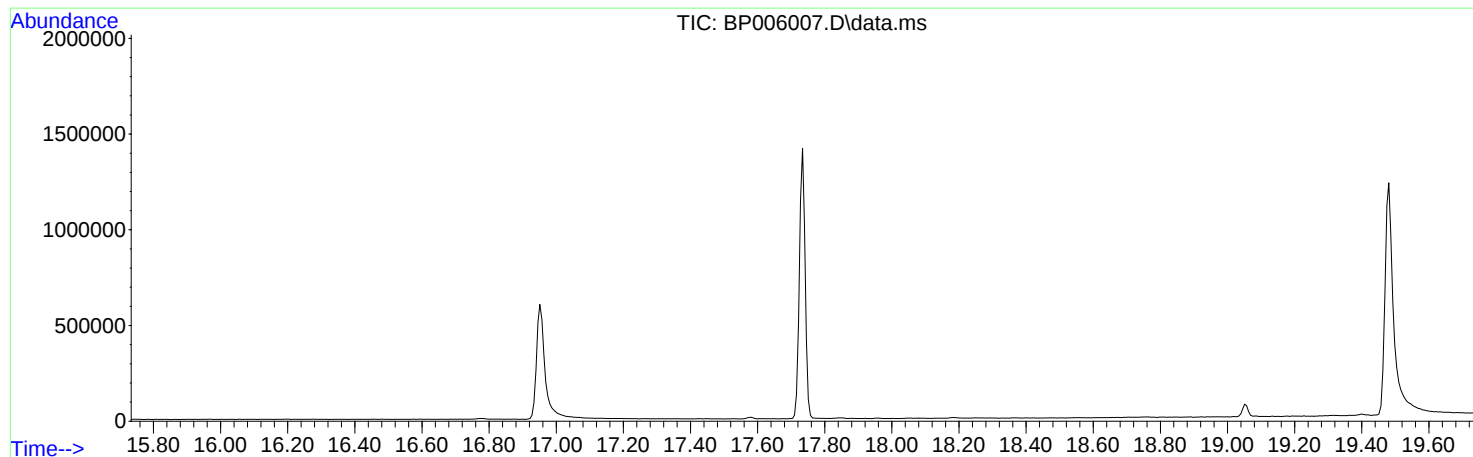




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.2	29523	PASS
68	69	0.00	2	2.0	752	PASS
69	198	0.00	100	33.6	37858	PASS
70	69	0.00	2	0.6	209	PASS
127	198	10	80	44.5	50187	PASS
197	198	0.00	2	0.3	306	PASS
198	198	100	100	100.0	112787	PASS
199	198	5	9	6.8	7616	PASS
275	198	10	60	31.5	35533	PASS
365	198	1	100	5.5	6258	PASS
441	198	0.01	100	28.7	32339	PASS
442	442	100	100	100.0	207829	PASS
443	442	15	24	19.5	40461	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062221\
 Data File : BP006007.D
 Acq On : 22 Jun 2021 15:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 22 17:49:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 11:35:30 2021
 Response via : Initial Calibration

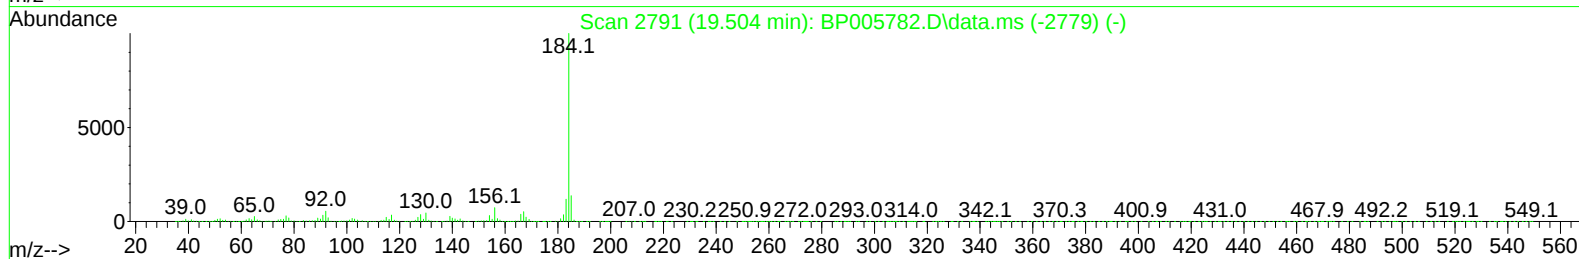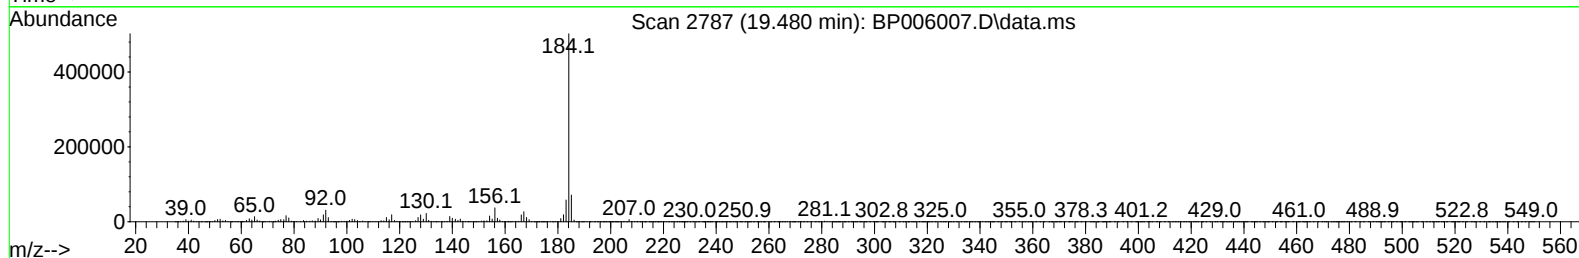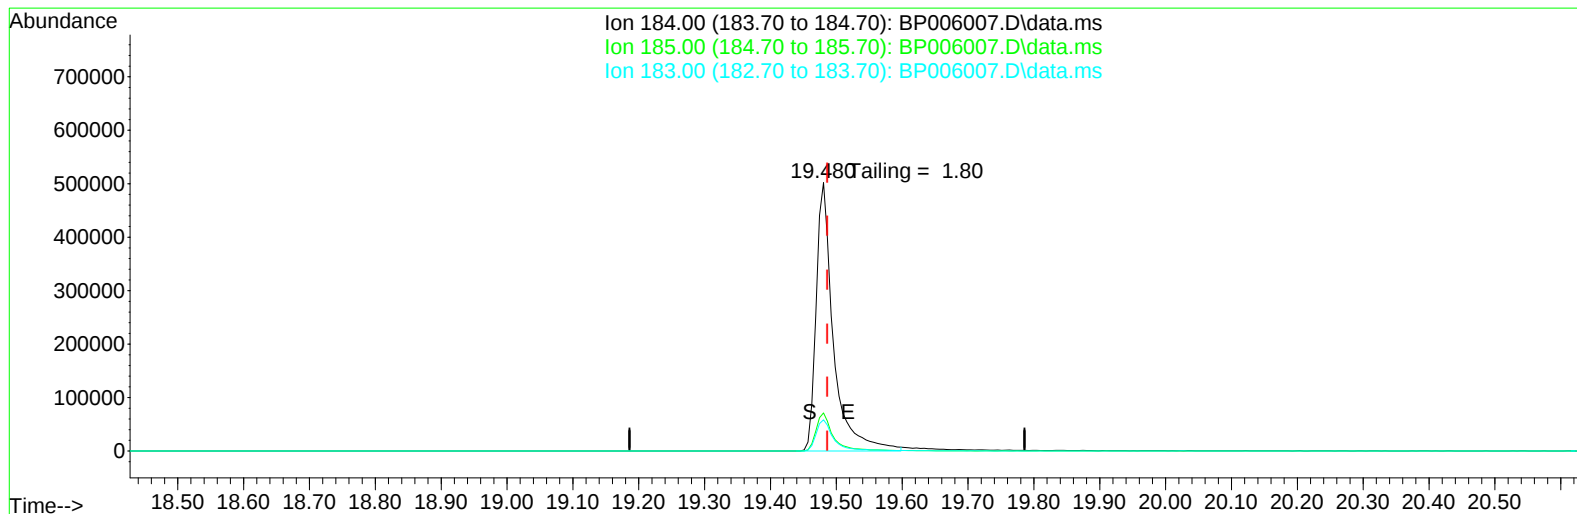

TIC: BP006007.D\data.ms

(77) Benzidine

19.480min (-0.006) 1010967.08 ng




response 925593

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.19
183.00	11.90	11.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062221\
Data File : BP006007.D
Acq On : 22 Jun 2021 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 22 17:49:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 11:35:30 2021
Response via : Initial Calibration

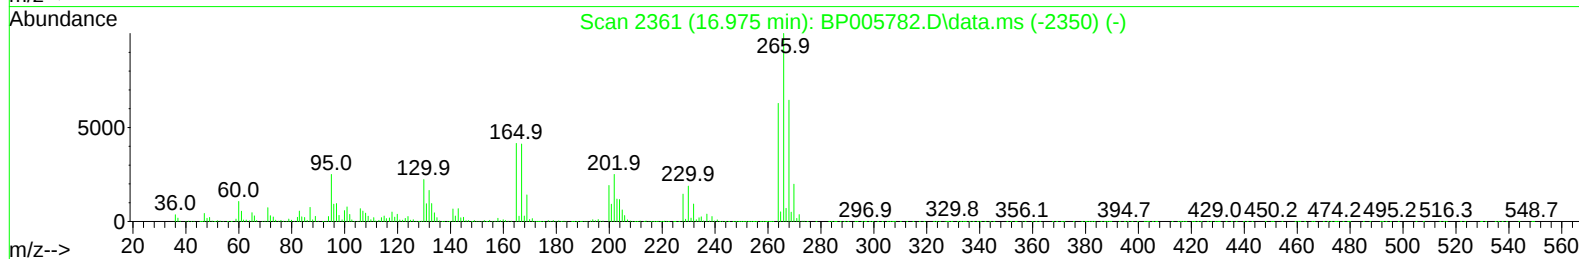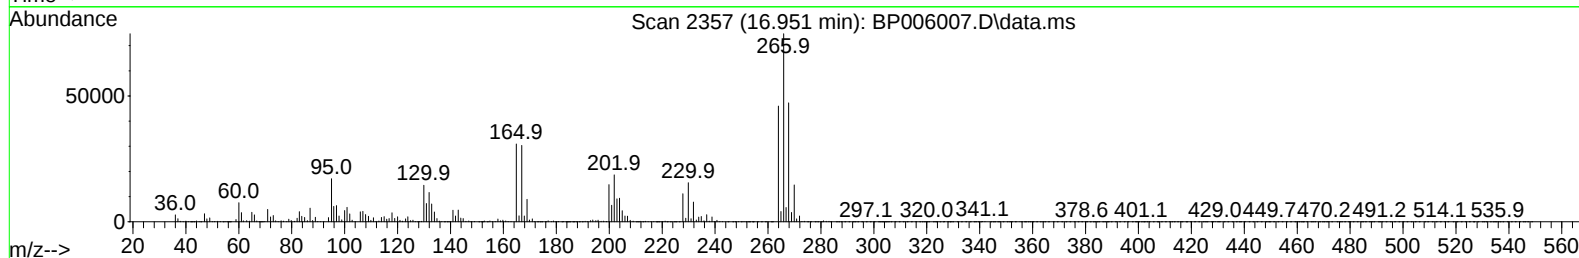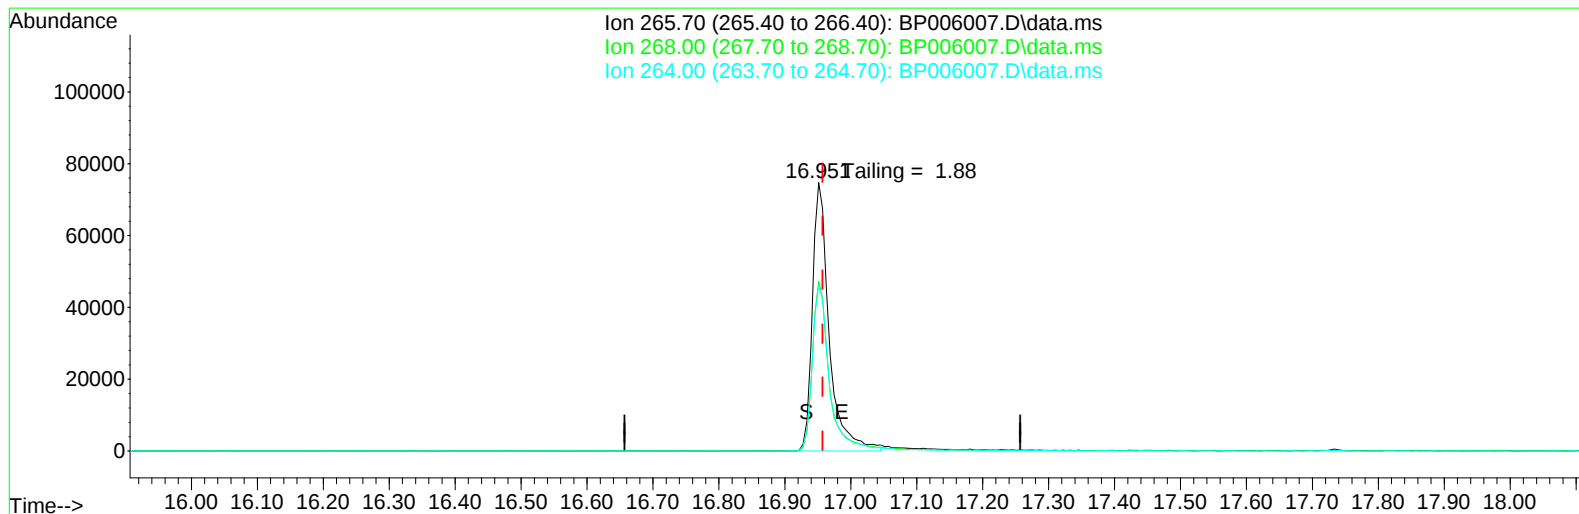

TIC: BP006007.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.006) 720076.02 ng

response 135516

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.26
264.00	62.90	61.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/22/2021	BNA_P	BP006007.D
Compound Name	Response	Retention Time
DDT	461824	20.67
DDD	9381	20.24
DDE	2117	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11498	473322	2.43