
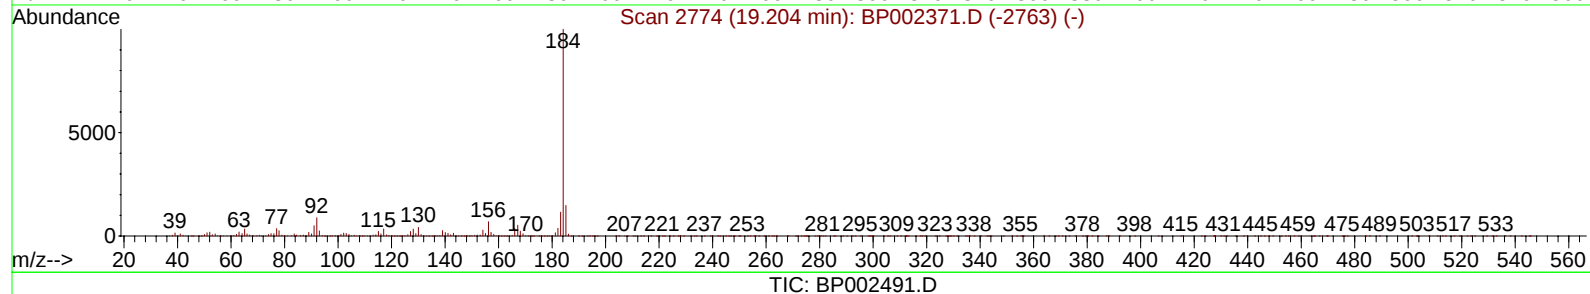
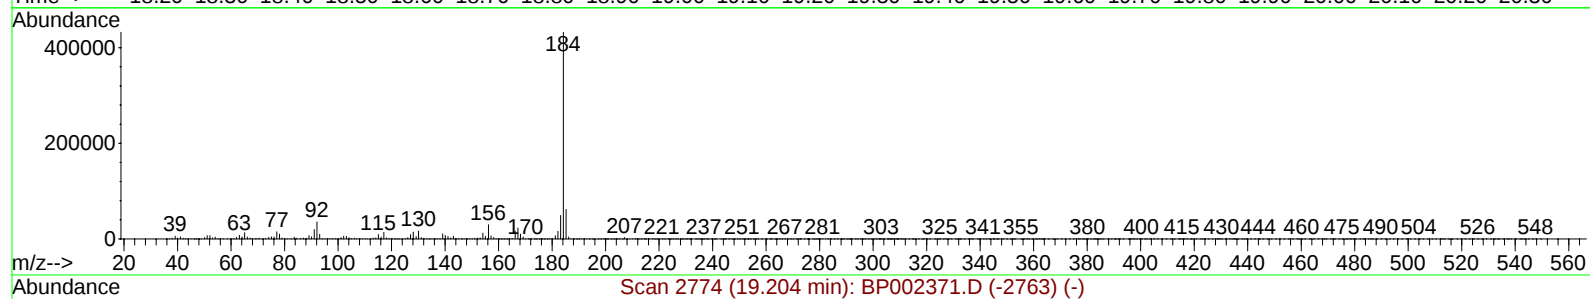


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062320\
 Data File : BP002491.D
 Acq On : 23 Jun 2020 08:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 16:56:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

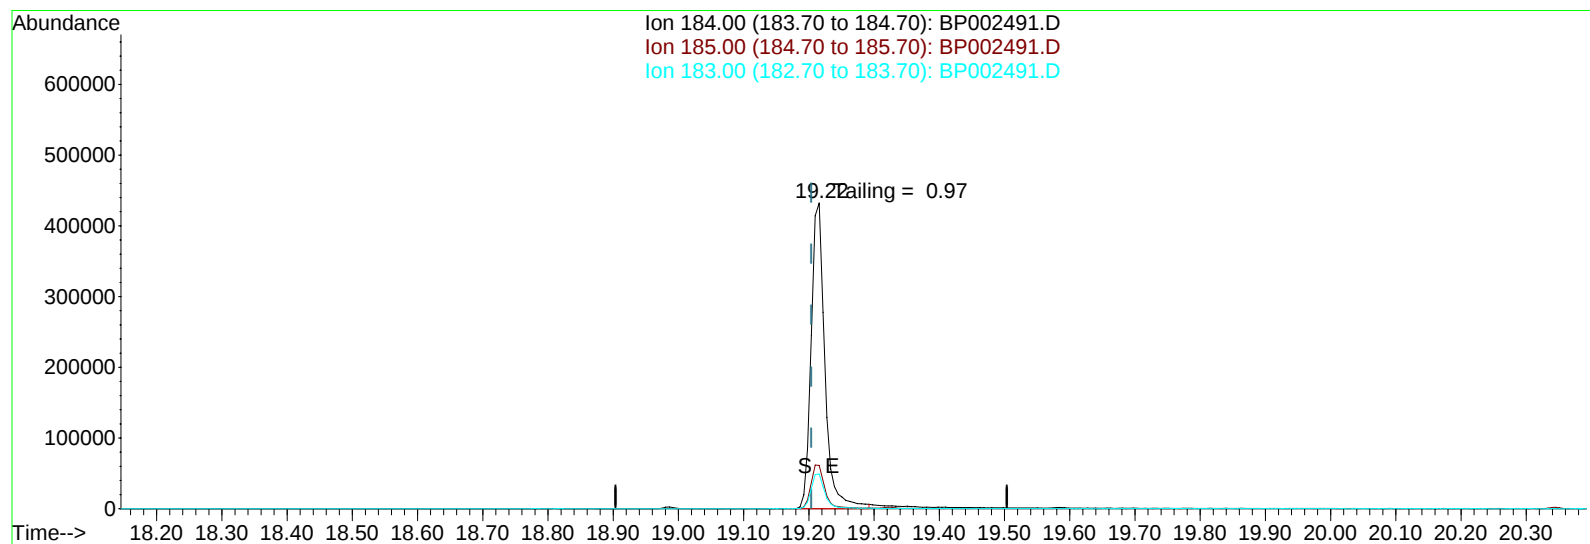

(77) Benzidine




19.216min (+0.012) 1875.42ng

response 651100

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.21
183.00	11.50	11.37
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062320\
Data File : BP002491.D
Acq On : 23 Jun 2020 08:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 16:56:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

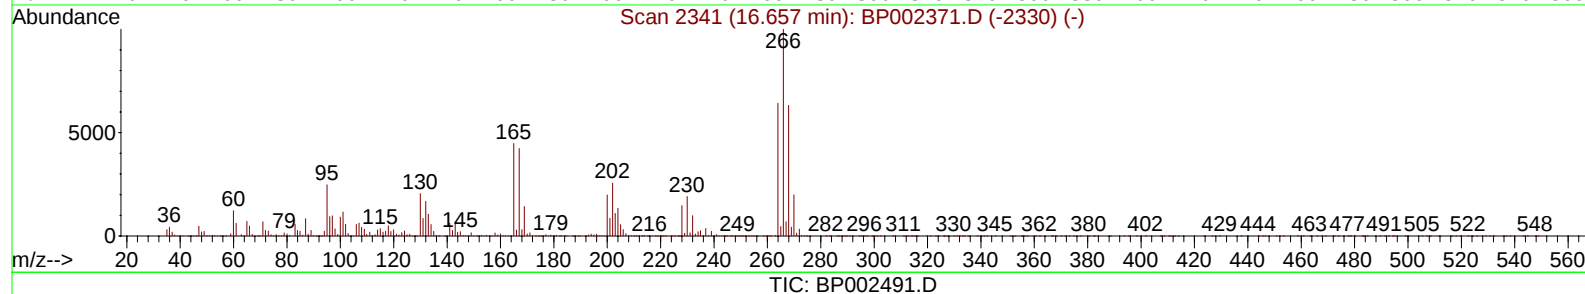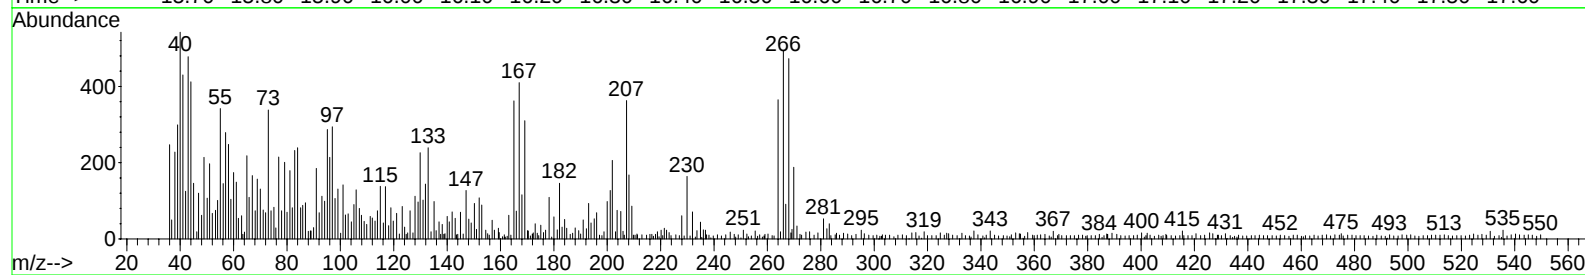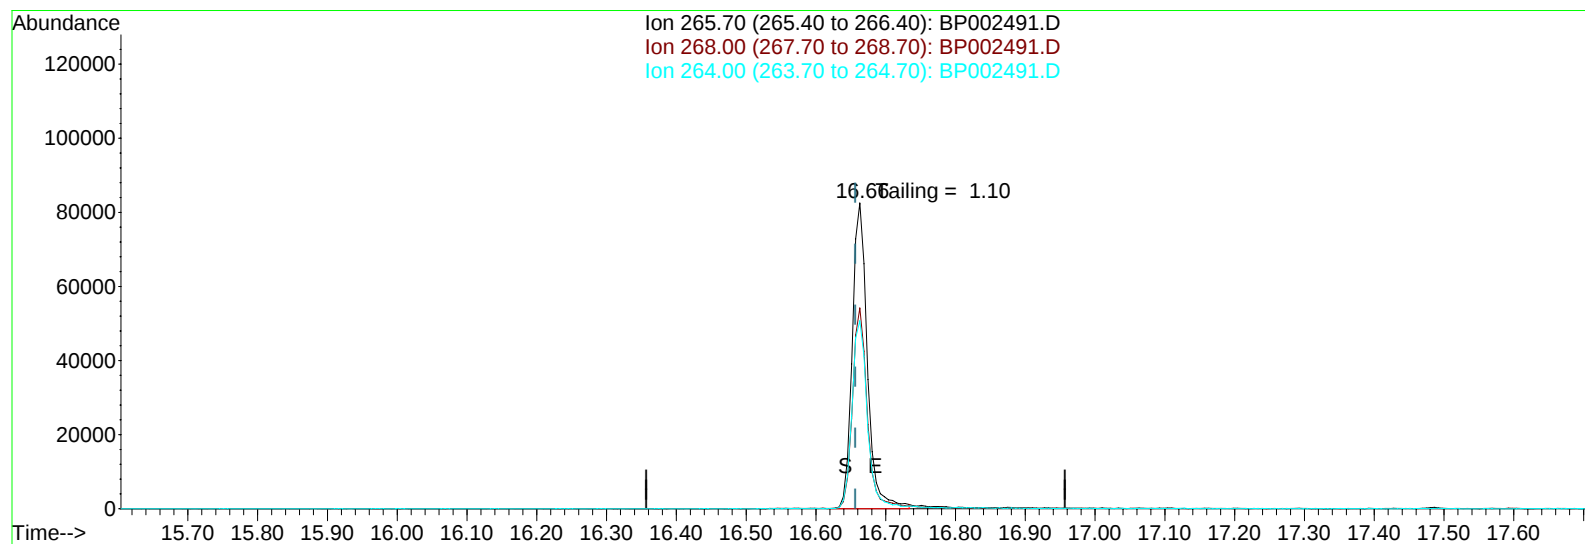

(70) Pentachlorophenol (C)

16.634min (-0.023) 24.37ng m

response 236

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	95.75#
264.00	64.20	73.89
0.00	0.00	0.00