
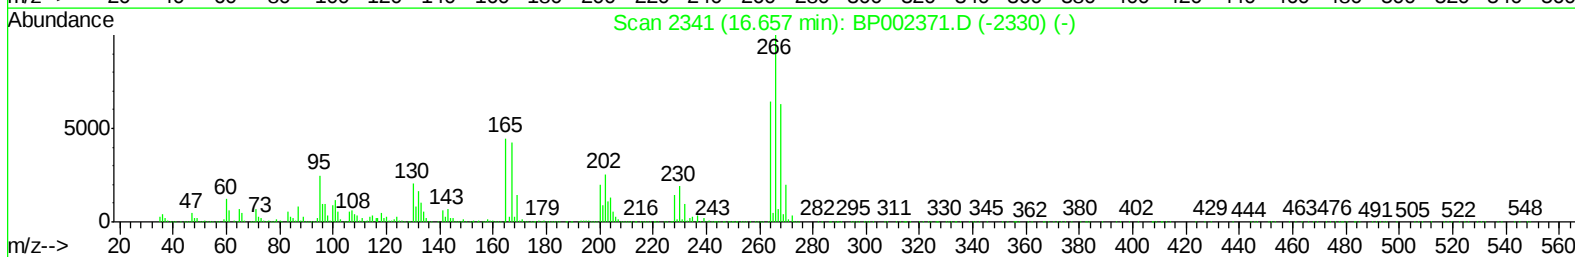
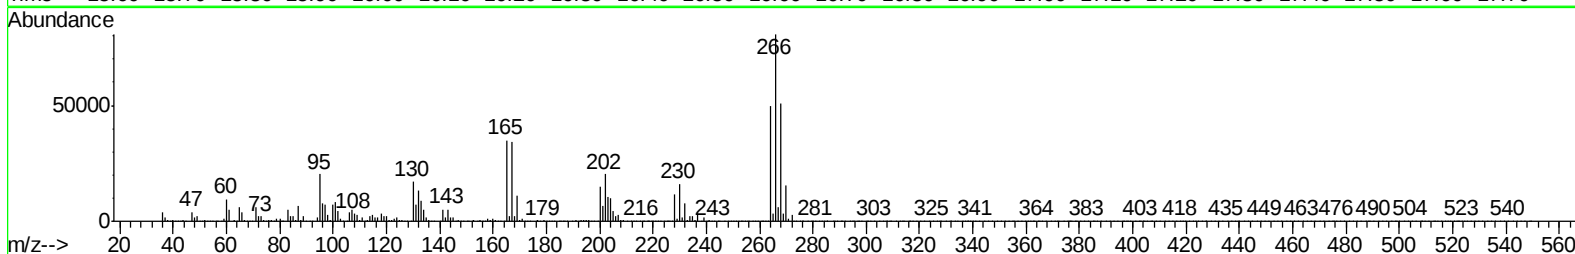


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062320\
Data File : BP002508.D
Acq On : 23 Jun 2020 18:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 00:54:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

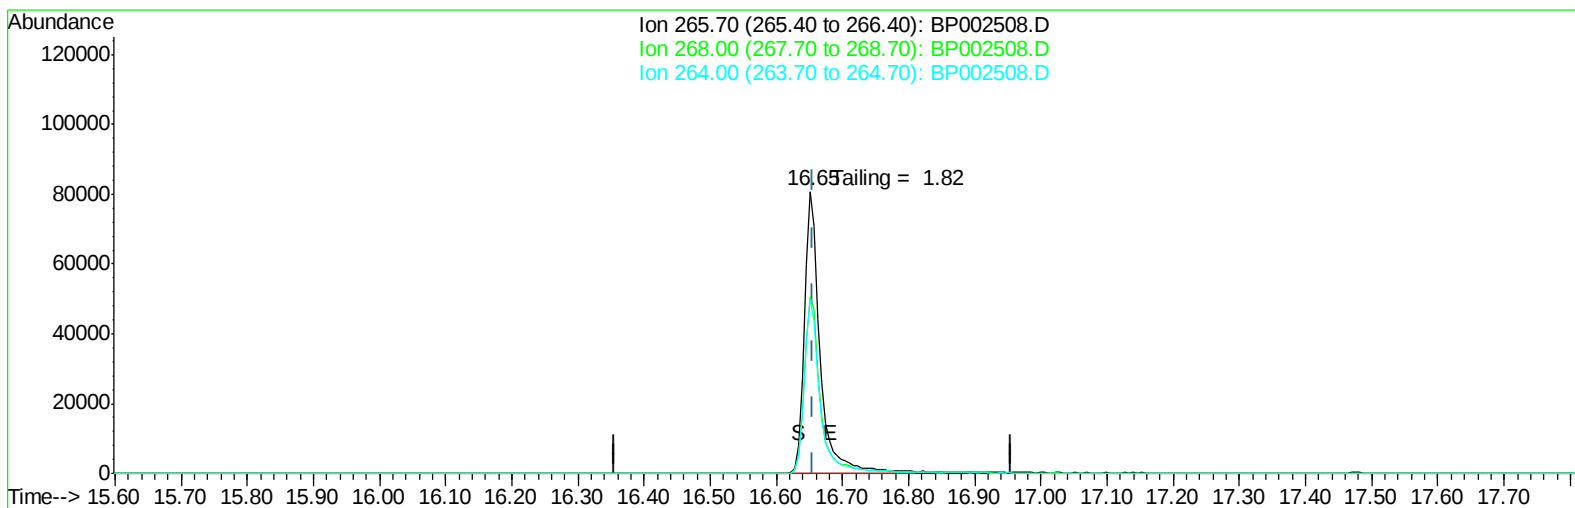

TIC: BP002508.D

(70) Pentachlorophenol (C)




16.651min (-0.005) 225080.23ng

response 135365

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	62.90
264.00	64.20	61.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062320\
Data File : BP002508.D
Acq On : 23 Jun 2020 18:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 00:54:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

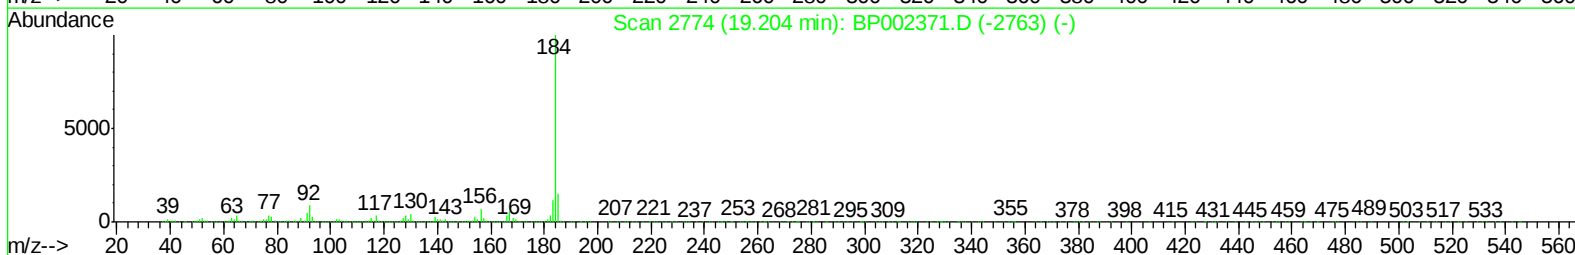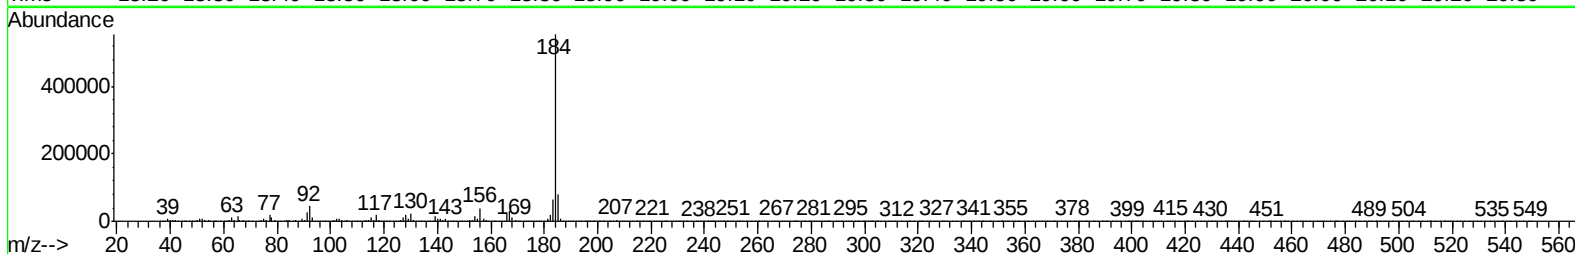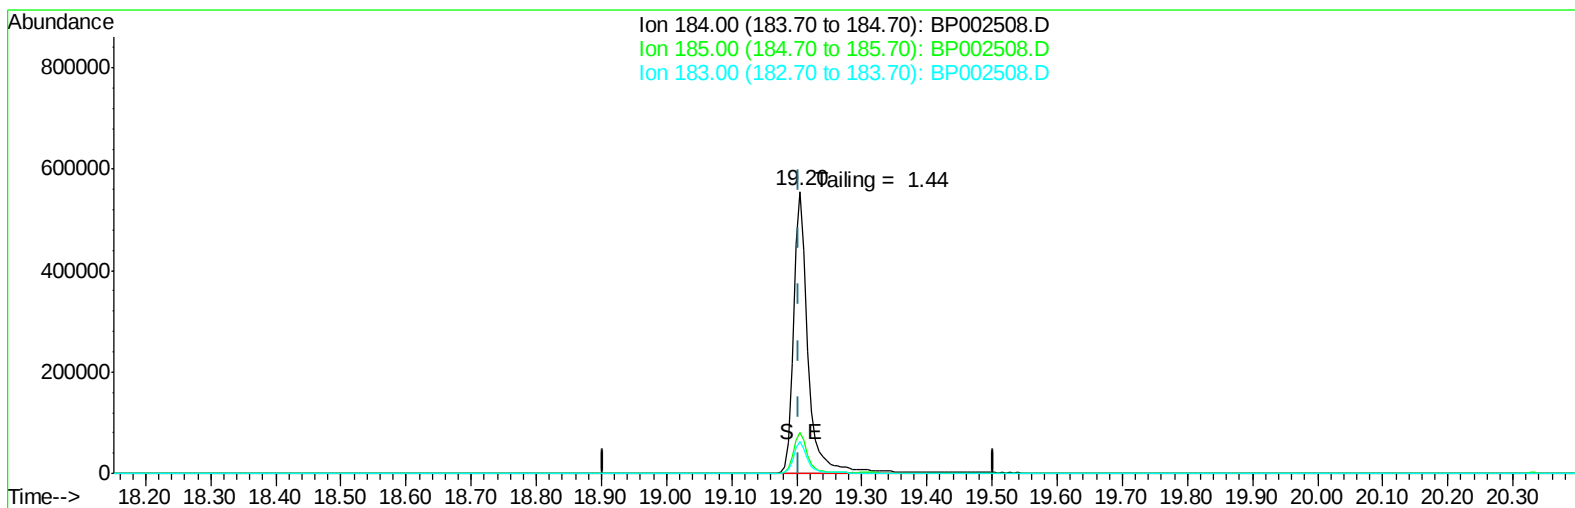

TIC: BP002508.D

(77) Benzidine

19.204min (+0.000) 444524.85ng

response 864164

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.64
183.00	11.50	11.36
0.00	0.00	0.00