


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP062320\
 Data File : BP002491.D
 Acq On : 23 Jun 2020 08:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

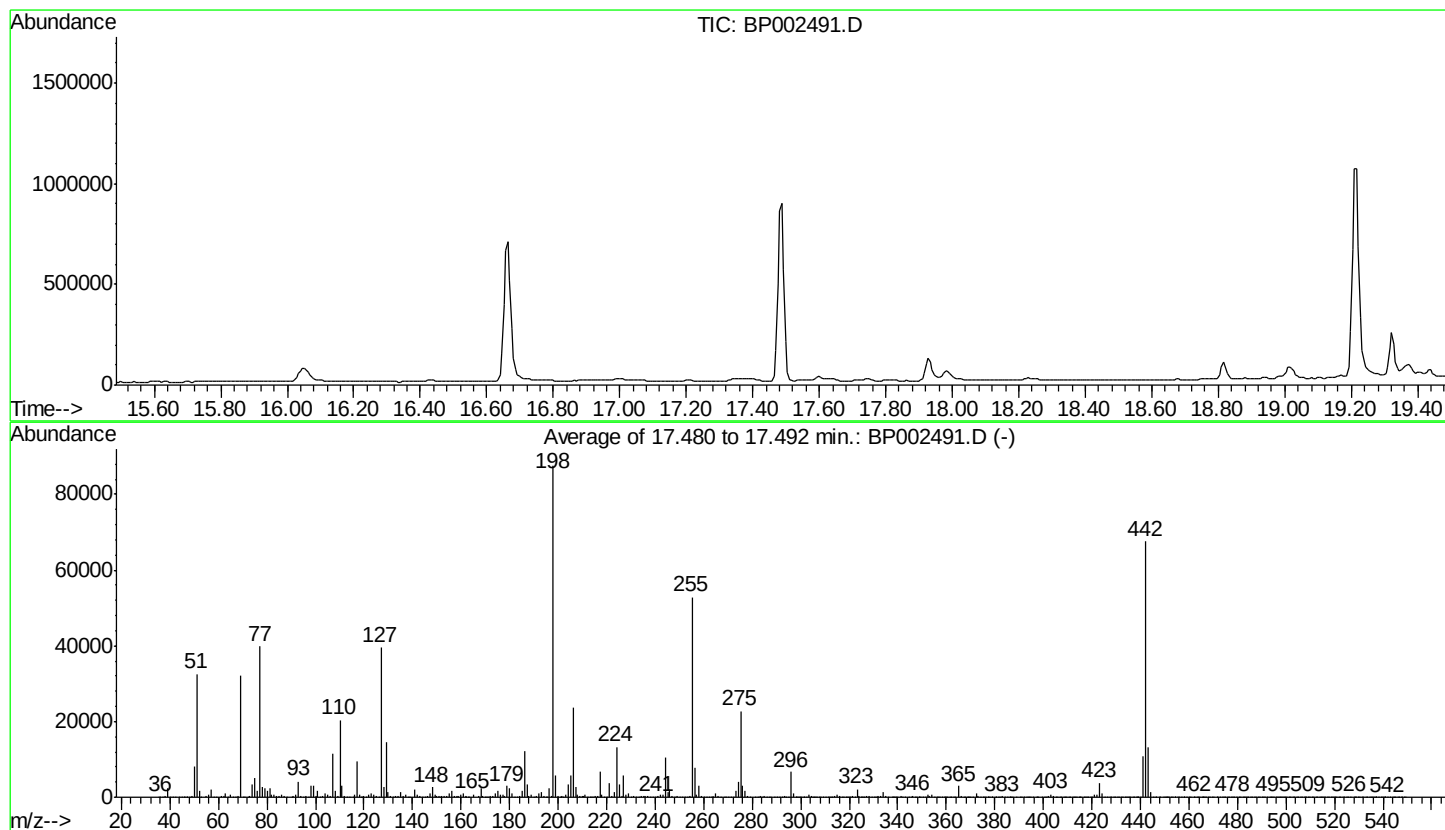

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	32611	PASS
68	69	0.00	2	1.5	473	PASS
69	198	0.00	100	36.7	32103	PASS
70	69	0.00	2	0.4	133	PASS
127	198	10	80	45.0	39435	PASS
197	198	0.00	2	0.4	318	PASS
198	198	100	100	100.0	87585	PASS
199	198	5	9	6.4	5630	PASS
275	198	10	60	26.0	22739	PASS
365	198	1	100	3.3	2934	PASS
441	198	0.01	100	12.4	10843	PASS
442	198	50	100	77.1	67544	PASS
443	442	15	24	19.4	13122	PASS