
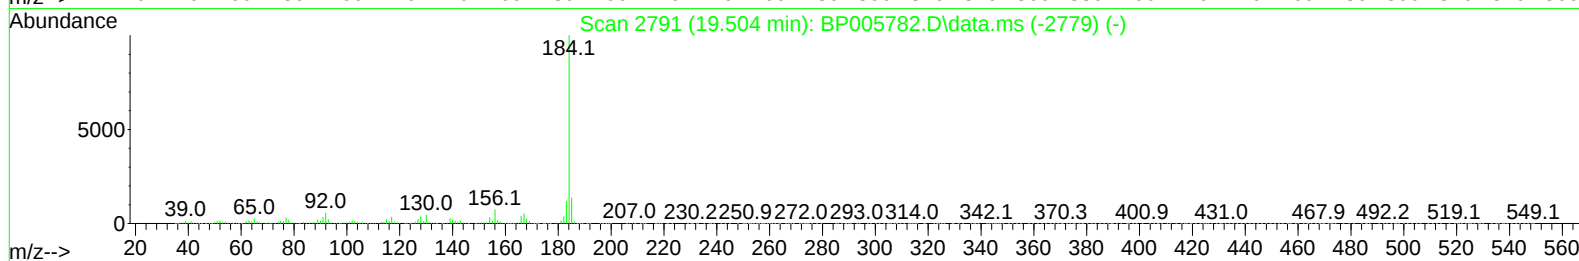
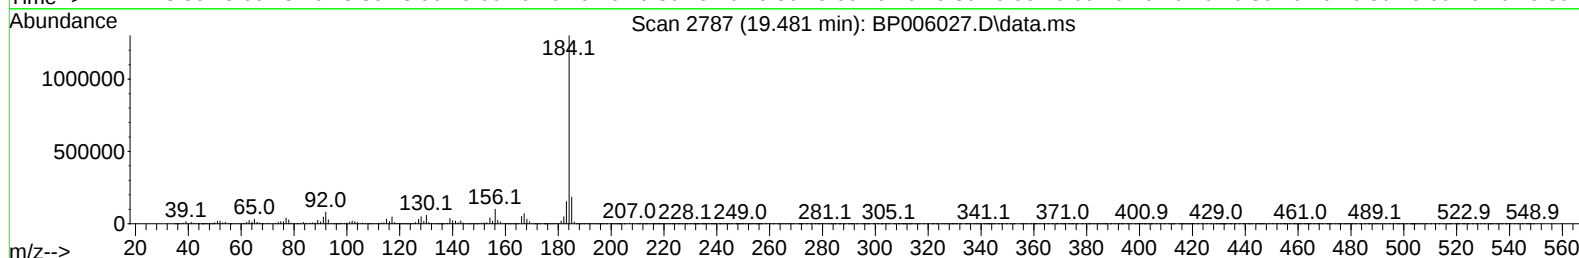


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062321\
Data File : BP006027.D
Acq On : 23 Jun 2021 09:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 11:22:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 22 17:52:38 2021
Response via : Initial Calibration

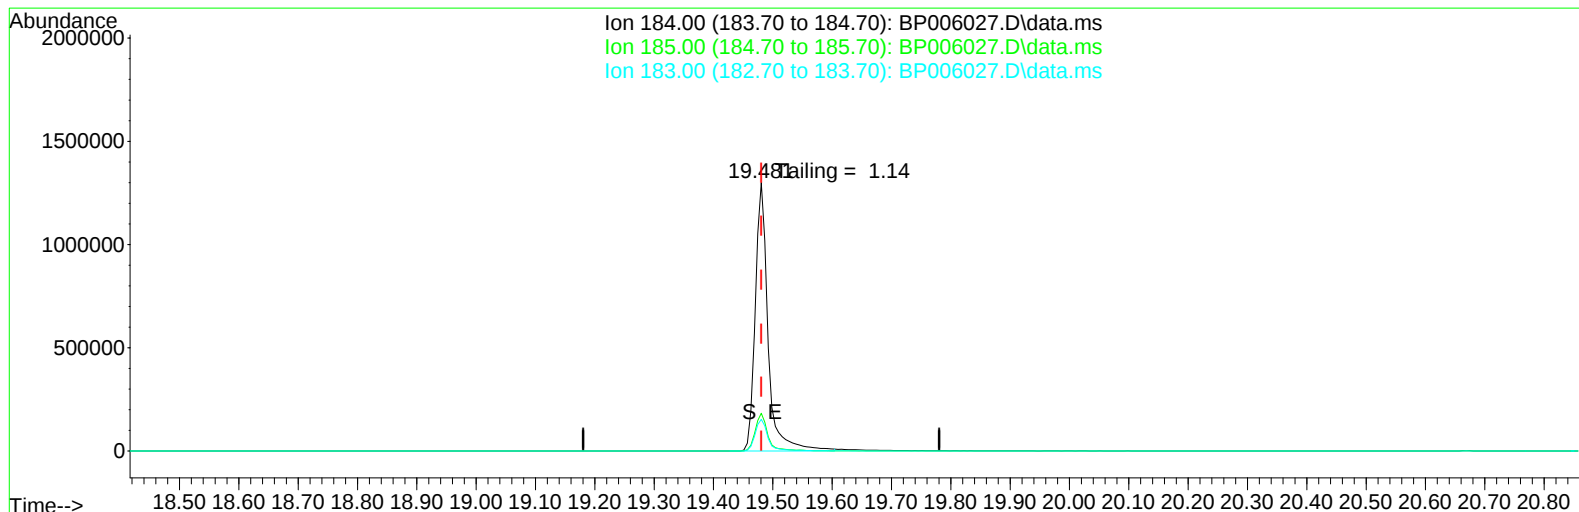

TIC: BP006027.D\data.ms

(77) Benzidine




19.481min (-0.000) 551624.94 ng m

response 1997209

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.10
183.00	11.90	11.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062321\
 Data File : BP006027.D
 Acq On : 23 Jun 2021 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 11:22:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 22 17:52:38 2021
 Response via : Initial Calibration

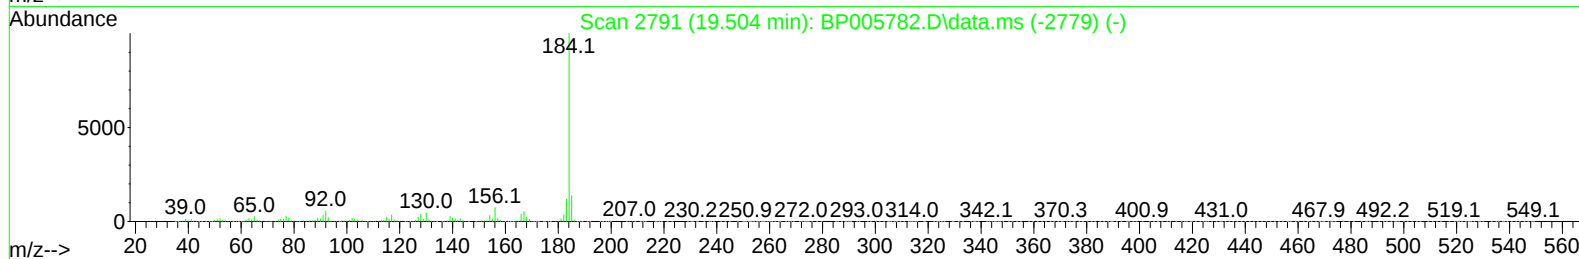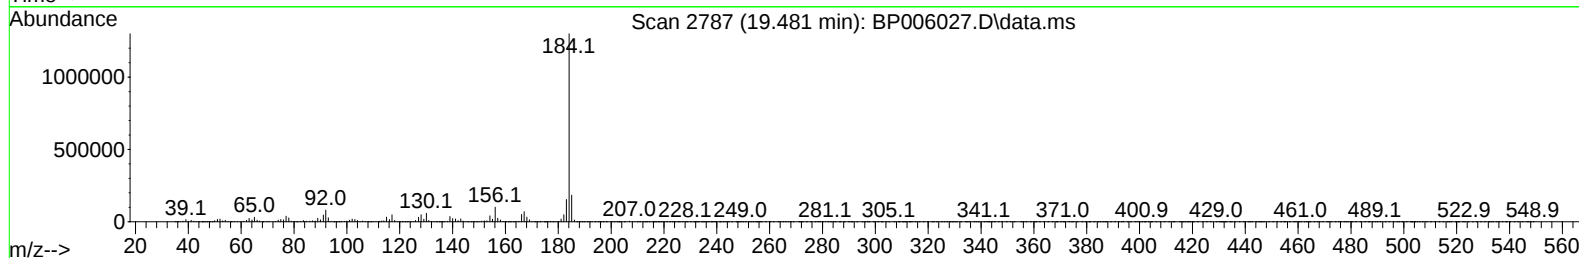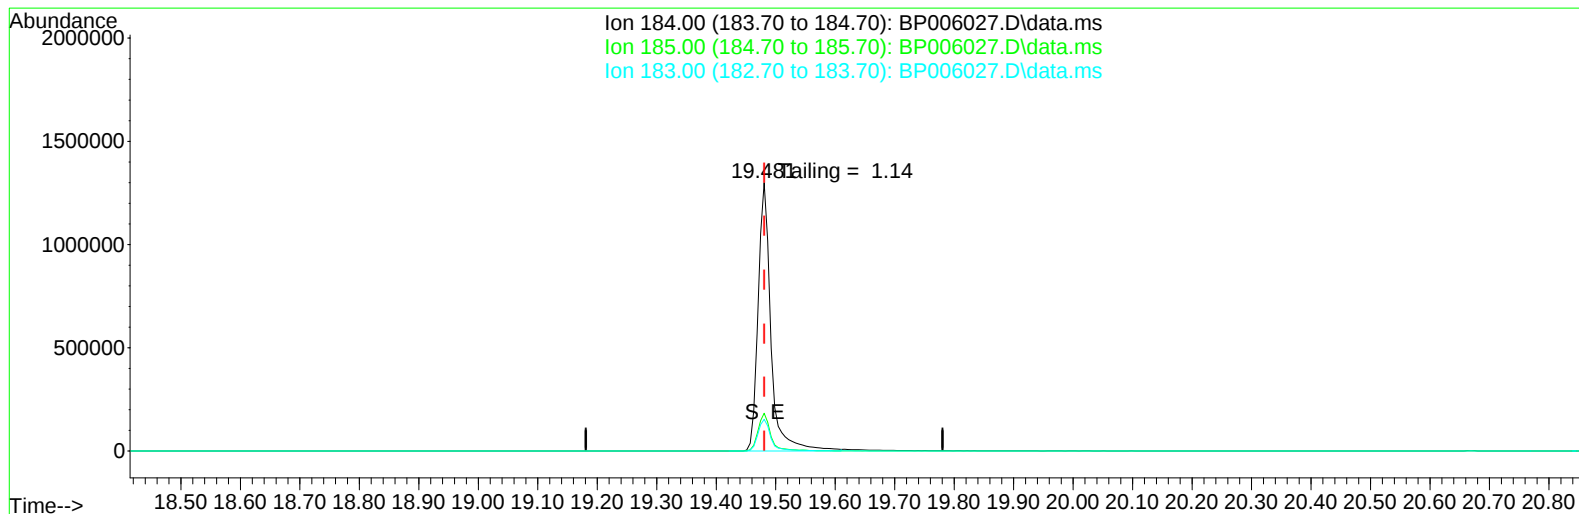

TIC: BP006027.D\data.ms

(77) Benzidine

19.481min (-0.000) 551514.74 ng m

response 1996810

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.10
183.00	11.90	11.79
0.00	0.00	0.00