
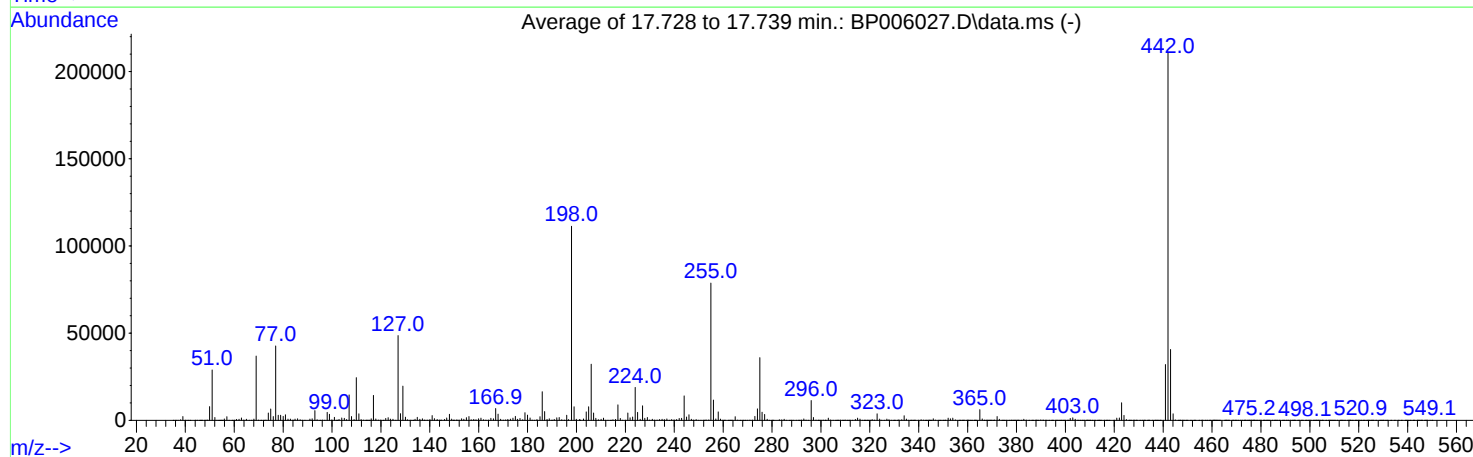


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062321\
 Data File : BP006027.D
 Acq On : 23 Jun 2021 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 22 17:52:38 2021

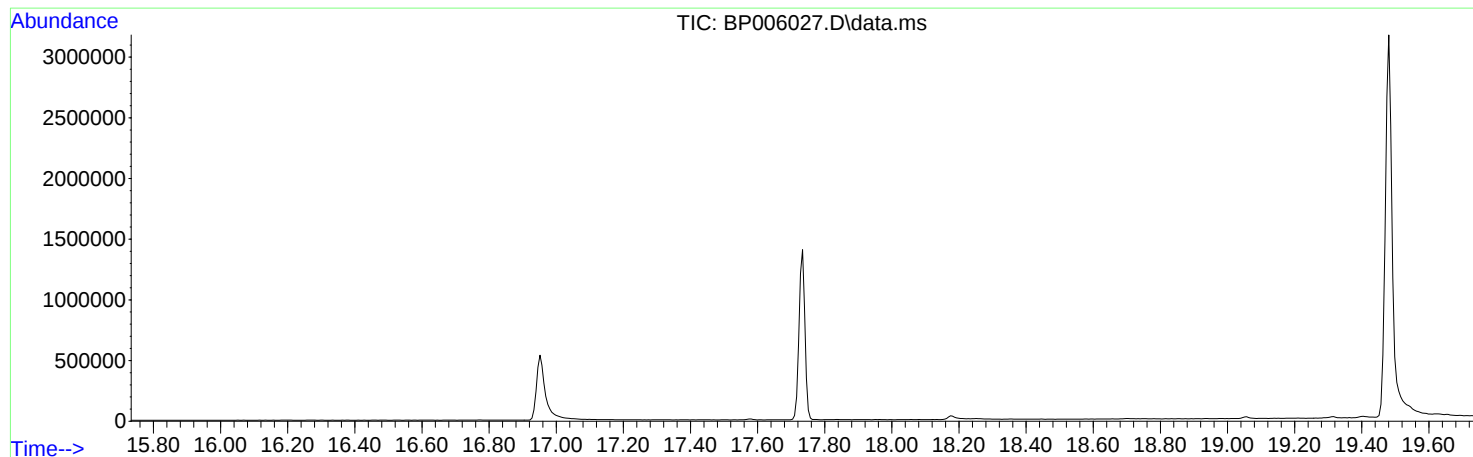




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	28936	PASS
68	69	0.00	2	1.9	709	PASS
69	198	0.00	100	33.2	36914	PASS
70	69	0.00	2	0.4	148	PASS
127	198	10	80	43.7	48631	PASS
197	198	0.00	2	0.4	487	PASS
198	198	100	100	100.0	111252	PASS
199	198	5	9	7.0	7832	PASS
275	198	10	60	32.3	35979	PASS
365	198	1	100	5.5	6139	PASS
441	198	0.01	100	28.8	32033	PASS
442	442	100	100	100.0	210880	PASS
443	442	15	24	19.3	40669	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062321\
 Data File : BP006027.D
 Acq On : 23 Jun 2021 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 23 11:22:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 22 17:52:38 2021
 Response via : Initial Calibration

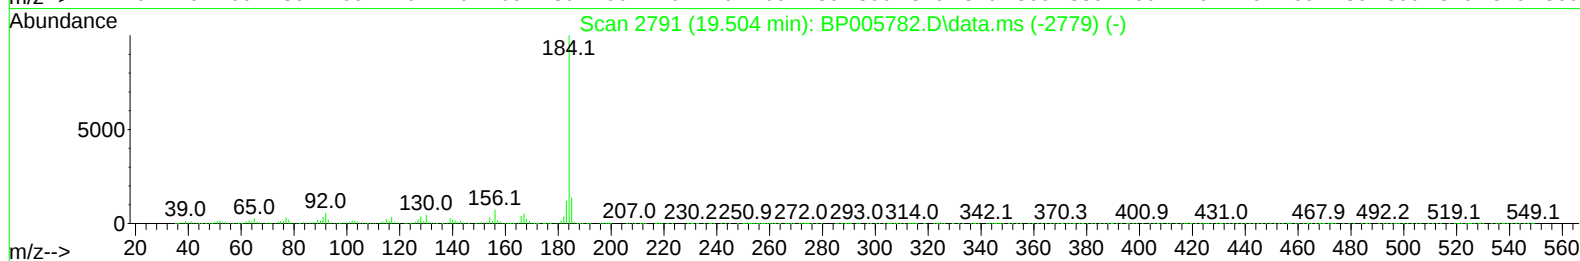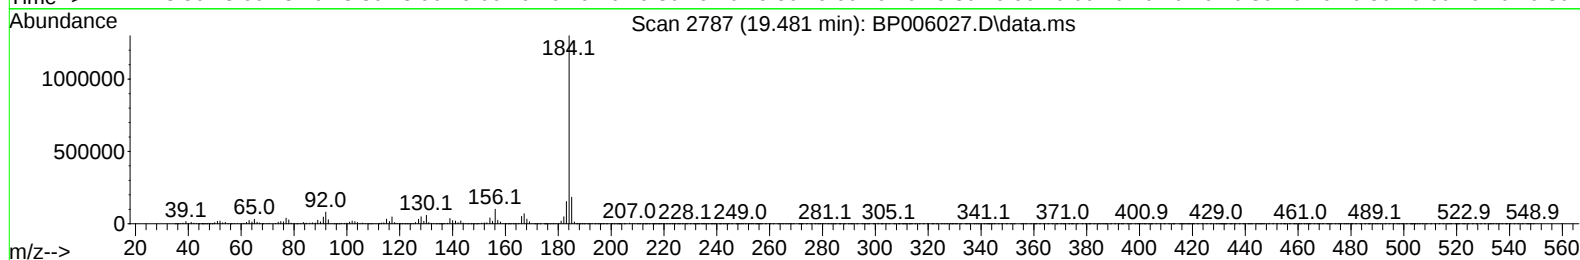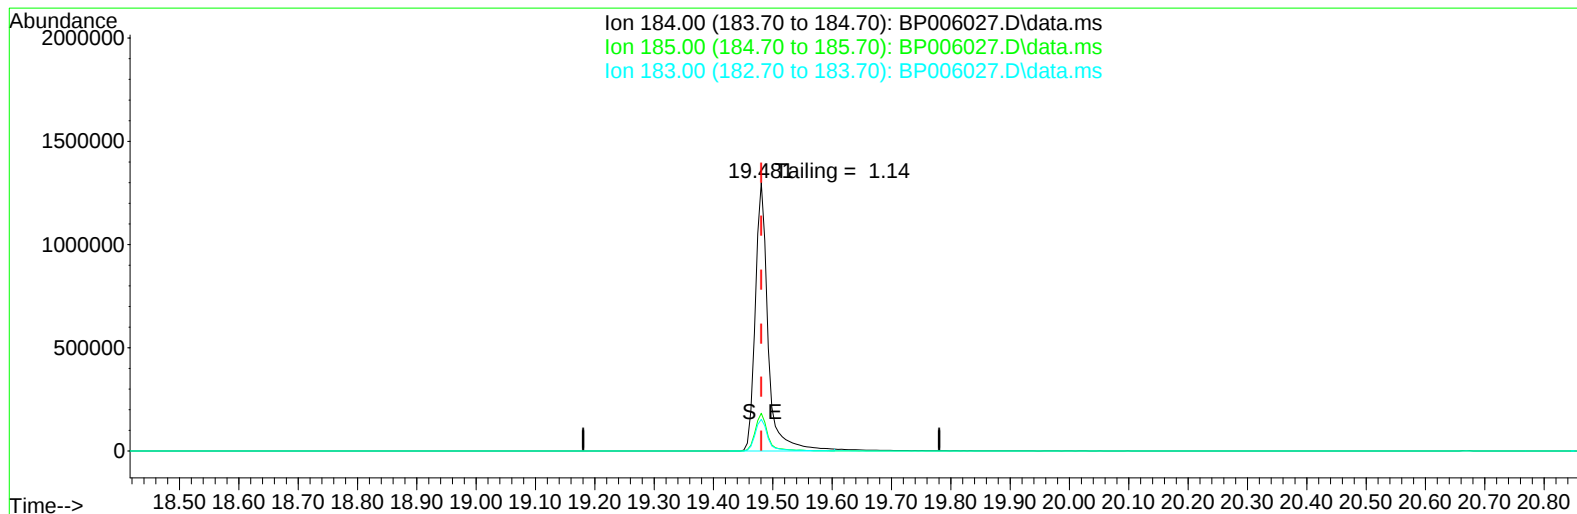

TIC: BP006027.D\data.ms

(77) Benzidine

19.481min (-0.000) 551624.94 ng m




response 1997209

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.10
183.00	11.90	11.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062321\
Data File : BP006027.D
Acq On : 23 Jun 2021 09:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 23 11:22:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 22 17:52:38 2021
Response via : Initial Calibration

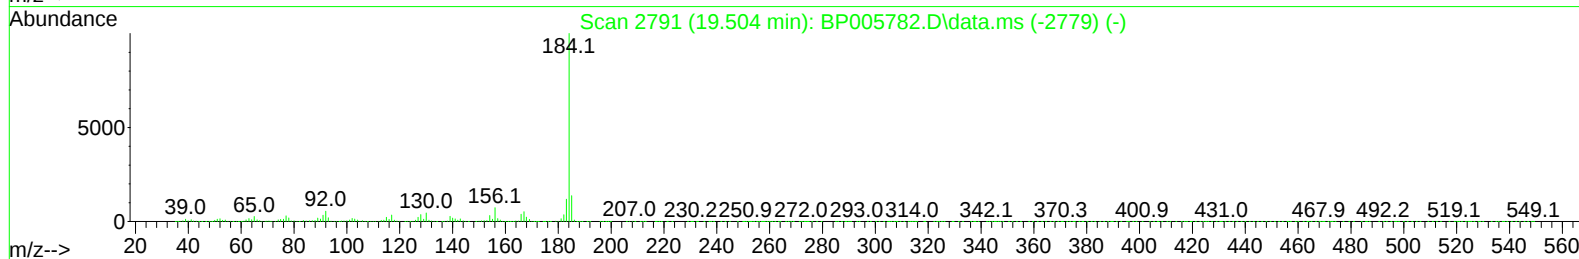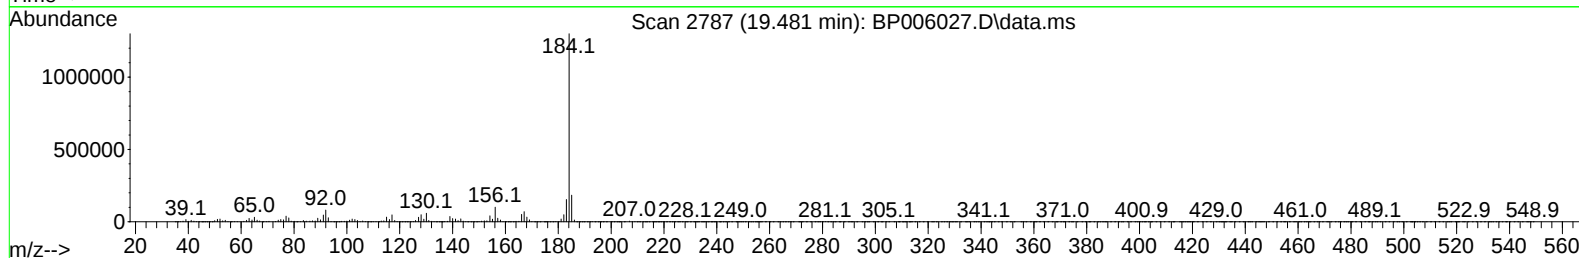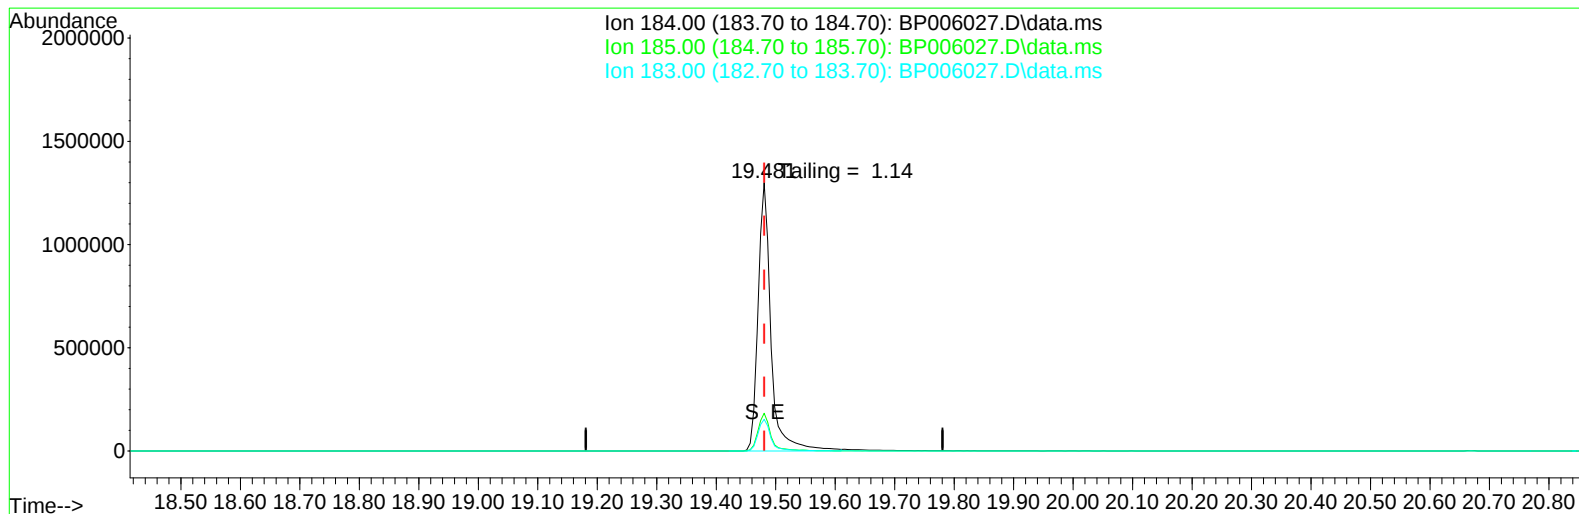

TIC: BP006027.D\data.ms

(77) Benzidine

19.481min (-0.000) 551514.74 ng m

response 1996810

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.10
183.00	11.90	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/23/2021	BNA_P	<u>BP006027.D</u>
Compound Name	Response	Retention Time
DDT	456862	20.66
DDD	5456	20.24
DDE	1606	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7062	463924	1.52