
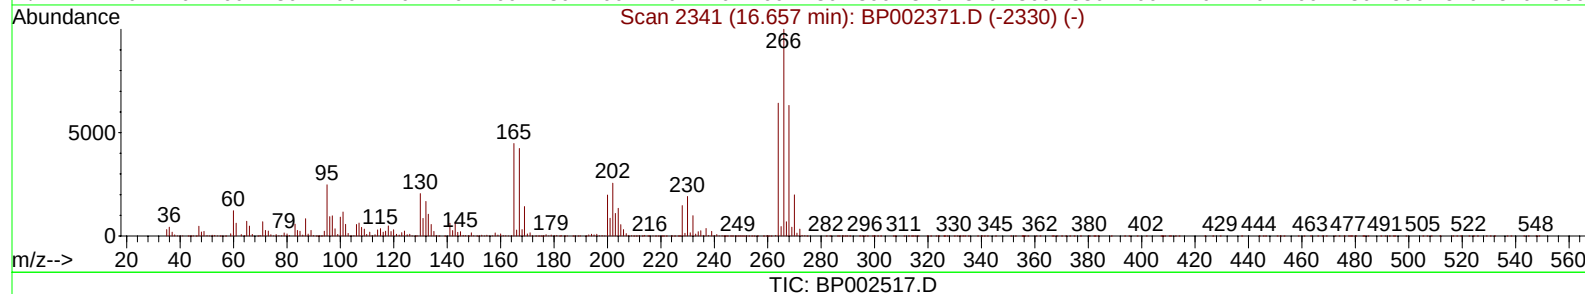
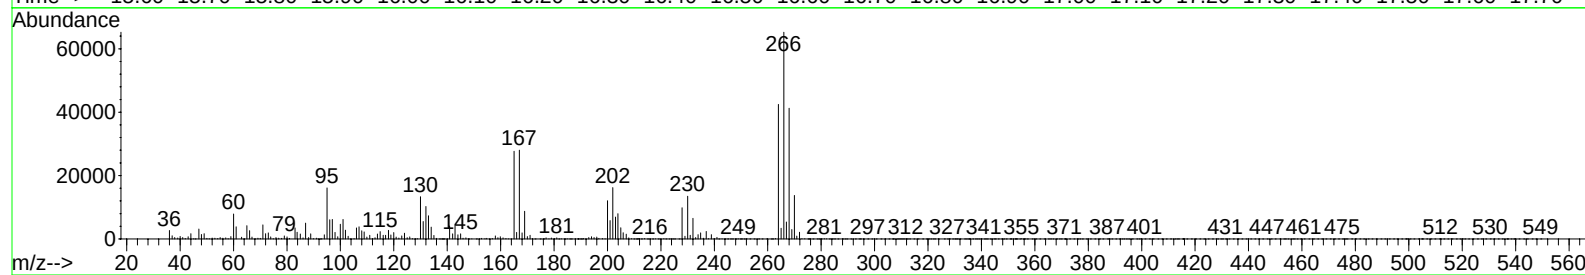


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062420\
 Data File : BP002517.D
 Acq On : 24 Jun 2020 11:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 18:32:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 24 13:54:06 2020
 Response via : Initial Calibration

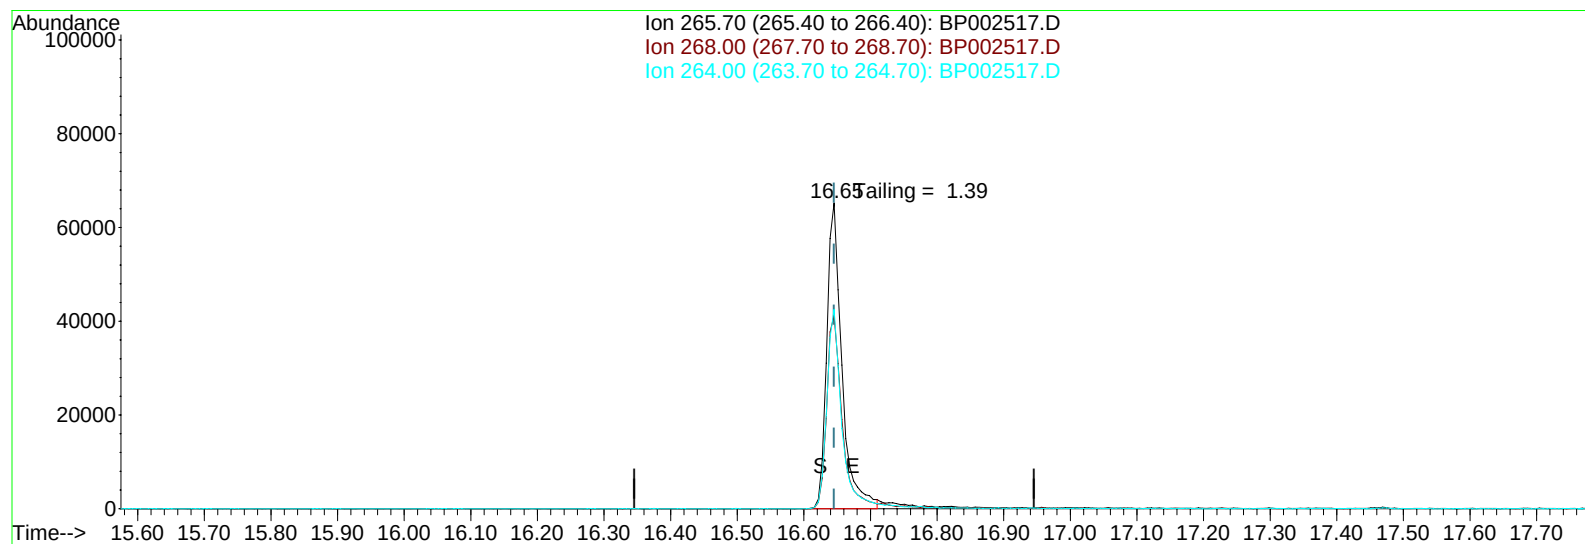

(70) Pentachlorophenol (C)




16.645min (+0.000) 443999.92ng

response 106810

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.23
264.00	64.80	65.13
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062420\
Data File : BP002517.D
Acq On : 24 Jun 2020 11:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 18:32:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 24 13:54:06 2020
Response via : Initial Calibration

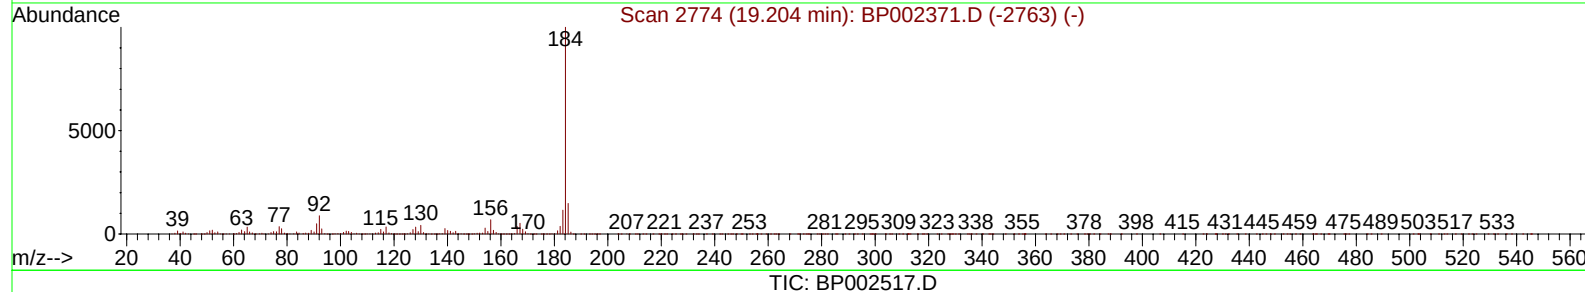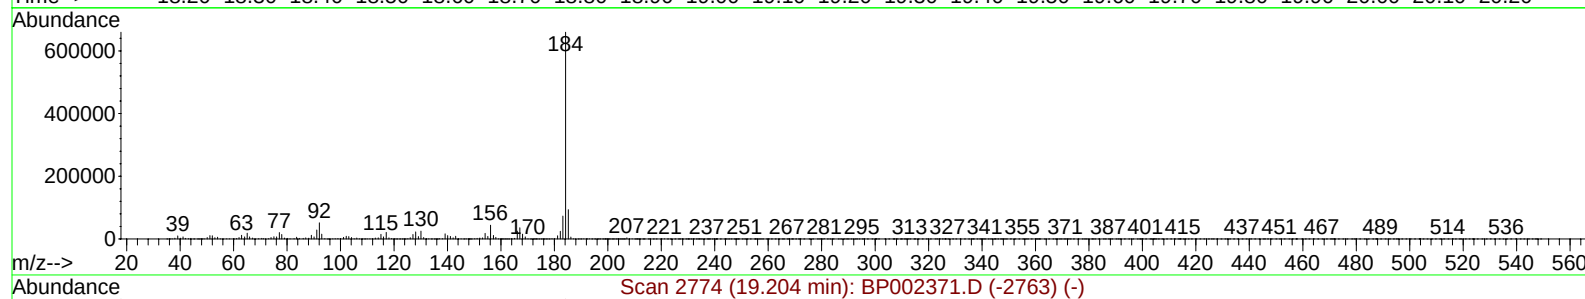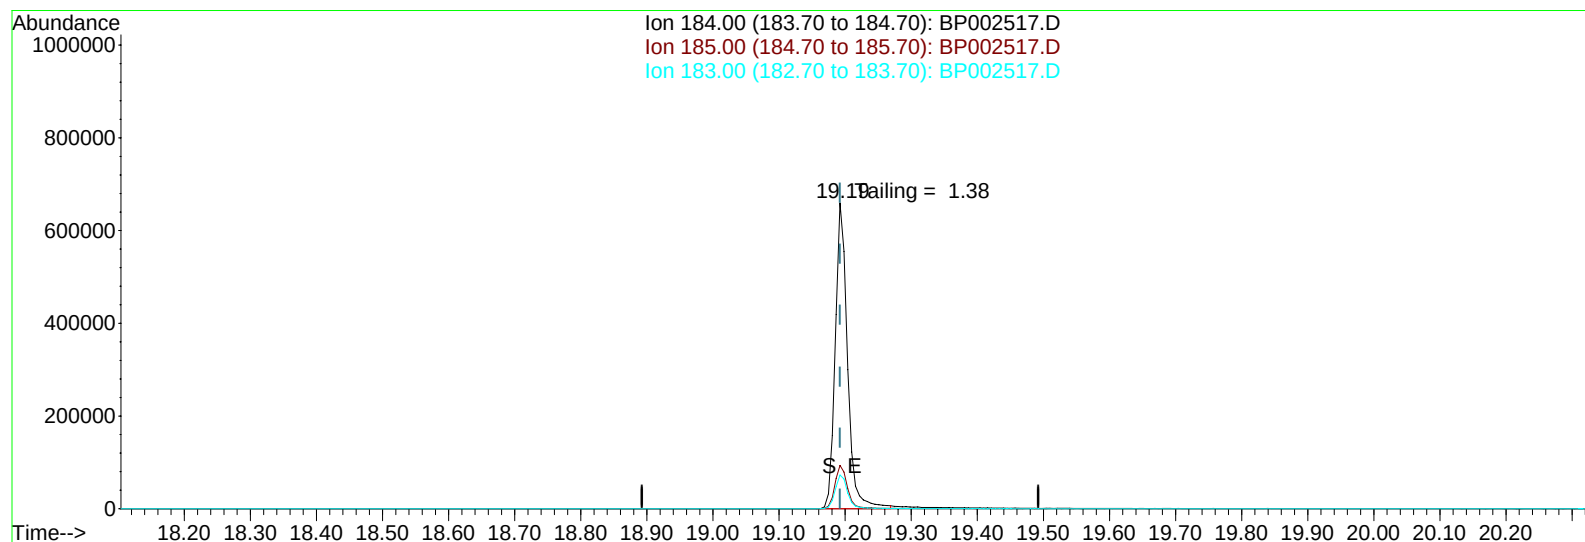

(77) Benzidine

19.192min (+0.000) 489751.89ng

response 864538

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.16
183.00	11.50	11.07
0.00	0.00	0.00