


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062420\
 Data File : BP002517.D
 Acq On : 24 Jun 2020 11:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 24 13:54:06 2020

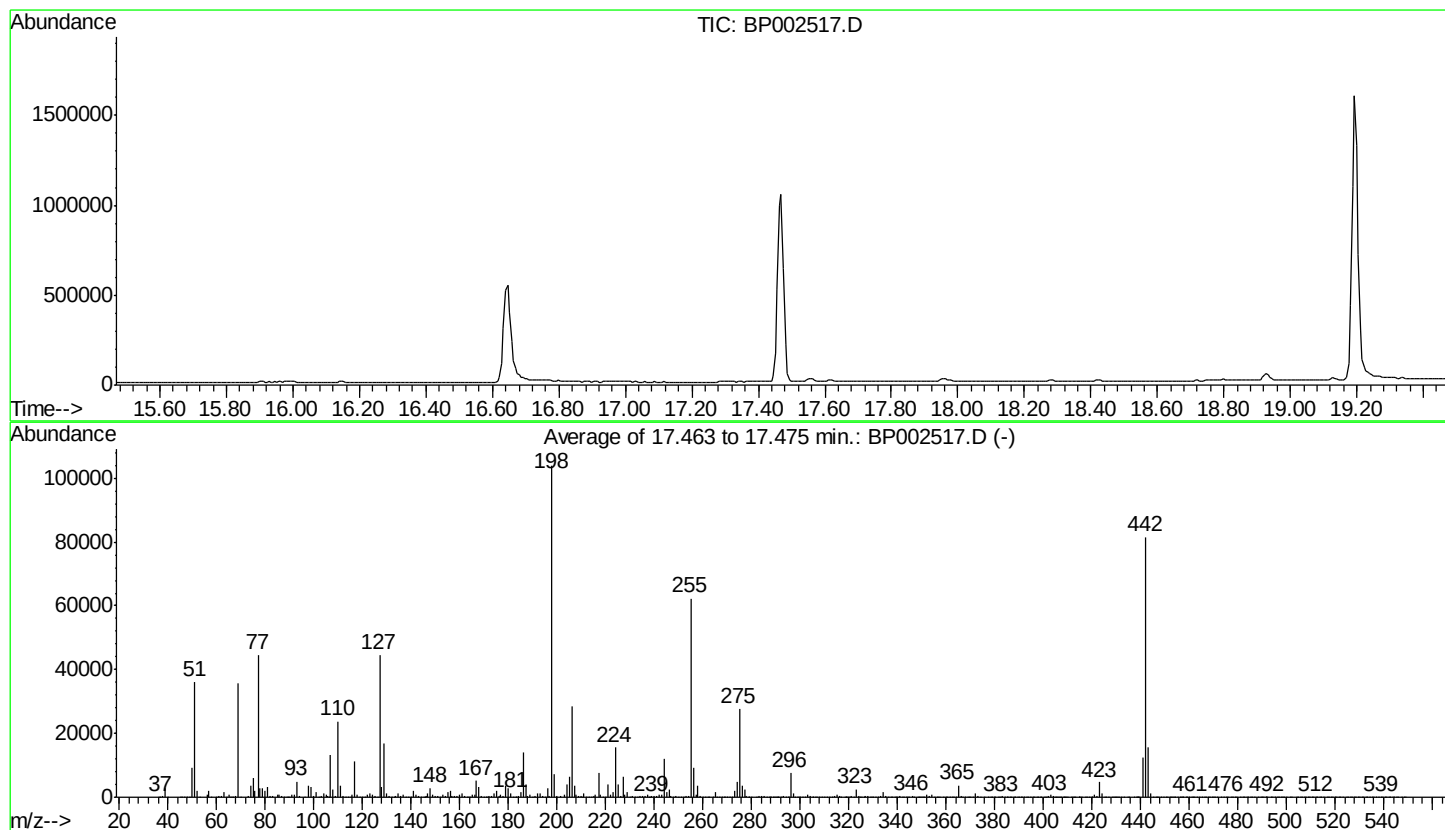

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	36115	PASS
68	69	0.00	2	1.4	492	PASS
69	198	0.00	100	34.4	35708	PASS
70	69	0.00	2	0.3	115	PASS
127	198	10	80	42.9	44550	PASS
197	198	0.00	2	0.3	289	PASS
198	198	100	100	100.0	103925	PASS
199	198	5	9	7.0	7257	PASS
275	198	10	60	26.6	27688	PASS
365	198	1	100	3.5	3617	PASS
441	198	0.01	100	11.9	12386	PASS
442	198	50	100	78.5	81629	PASS
443	442	15	24	19.2	15645	PASS