

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP0602421\
 Data File : BP006056.D
 Acq On : 24 Jun 2021 16:55
 Operator : CG/JU
 Sample : M2776-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 0339-DISCRETE-CORE-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	324	329	335	rBV	16418	25688	1.33%	0.168%
2	5.487	401	408	427	rBV	929866	1411909	73.09%	9.246%
3	7.093	668	681	696	rBV	850490	1446676	74.89%	9.473%
4	7.211	696	701	709	rVB	18510	33413	1.73%	0.219%
5	7.911	814	820	830	rBV	270467	424908	22.00%	2.782%
6	9.081	1009	1019	1037	rBV	462071	843805	43.68%	5.525%
7	10.516	1254	1263	1275	rBV2	21602	59220	3.07%	0.388%
8	10.716	1287	1297	1310	rBV	311482	558098	28.89%	3.655%
9	13.169	1706	1714	1733	rBV	987817	1490886	77.18%	9.763%
10	14.269	1894	1901	1909	rBV	11304	19847	1.03%	0.130%
11	14.540	1939	1947	1964	rVV	491655	731688	37.88%	4.791%
12	15.363	2077	2087	2095	rBV2	15666	33298	1.72%	0.218%
13	16.034	2191	2201	2221	rBV	1203156	1931666	100.00%	12.649%
14	17.286	2408	2414	2419	rBV	591609	857506	44.39%	5.615%
15	17.328	2419	2421	2430	rVV	86699	118186	6.12%	0.774%
16	17.422	2434	2437	2443	rVB	14810	25253	1.31%	0.165%
17	18.169	2557	2564	2567	rBV2	33123	64304	3.33%	0.421%
18	18.204	2567	2570	2574	rVB	22017	29720	1.54%	0.195%
19	18.345	2588	2594	2597	rBV3	31760	53964	2.79%	0.353%
20	19.292	2750	2755	2762	rBV	148908	202027	10.46%	1.323%
21	19.533	2794	2796	2805	rVB9	13905	21176	1.10%	0.139%
22	19.616	2807	2810	2811	rVV2	22757	26662	1.38%	0.175%
23	19.645	2811	2815	2823	rVB	187842	255915	13.25%	1.676%
24	19.833	2842	2847	2854	rBV	1586487	1833757	94.93%	12.008%
25	20.128	2894	2897	2901	rVB2	34886	43061	2.23%	0.282%
26	20.222	2910	2913	2917	rBV2	27533	33346	1.73%	0.218%
27	21.057	3052	3055	3058	rBV3	59043	76061	3.94%	0.498%
28	21.139	3066	3069	3075	rVB2	45679	66593	3.45%	0.436%
29	21.363	3101	3107	3111	rBV	876322	1251714	64.80%	8.197%
30	23.763	3509	3515	3529	rVB2	604663	1300909	67.35%	8.519%




Sum of corrected areas: 15271256

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
Data File : BP006056.D
Acq On : 24 Jun 2021 16:55
Operator : CG/JU
Sample : M2776-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
0339-DISCRETE-CORE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

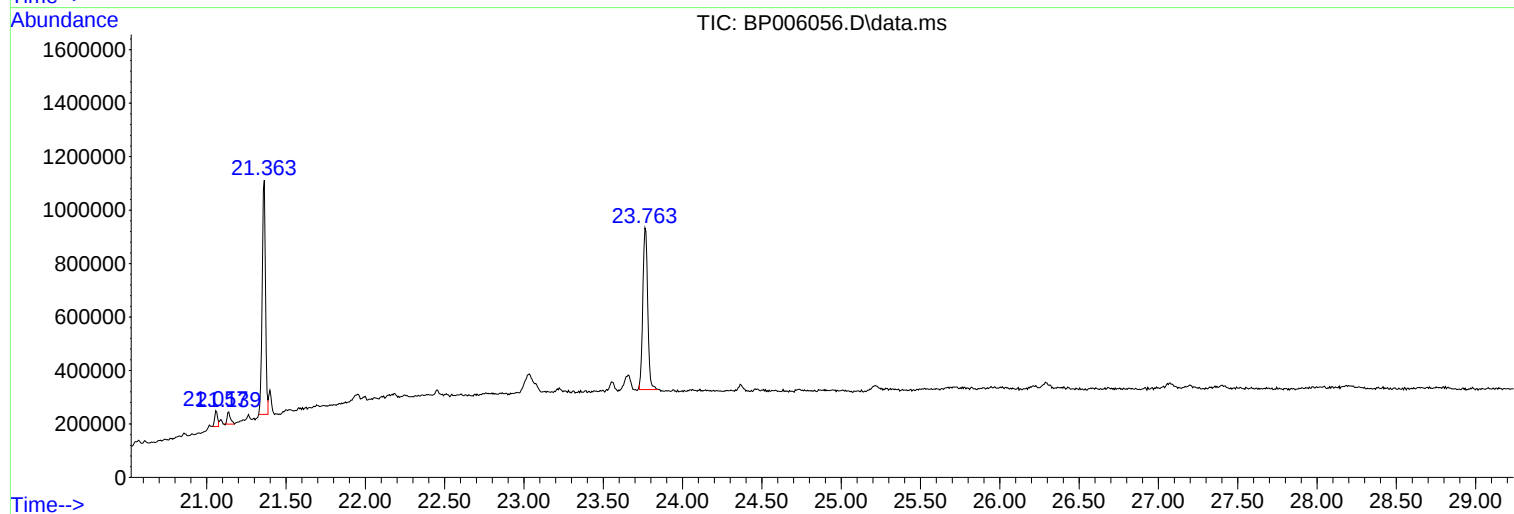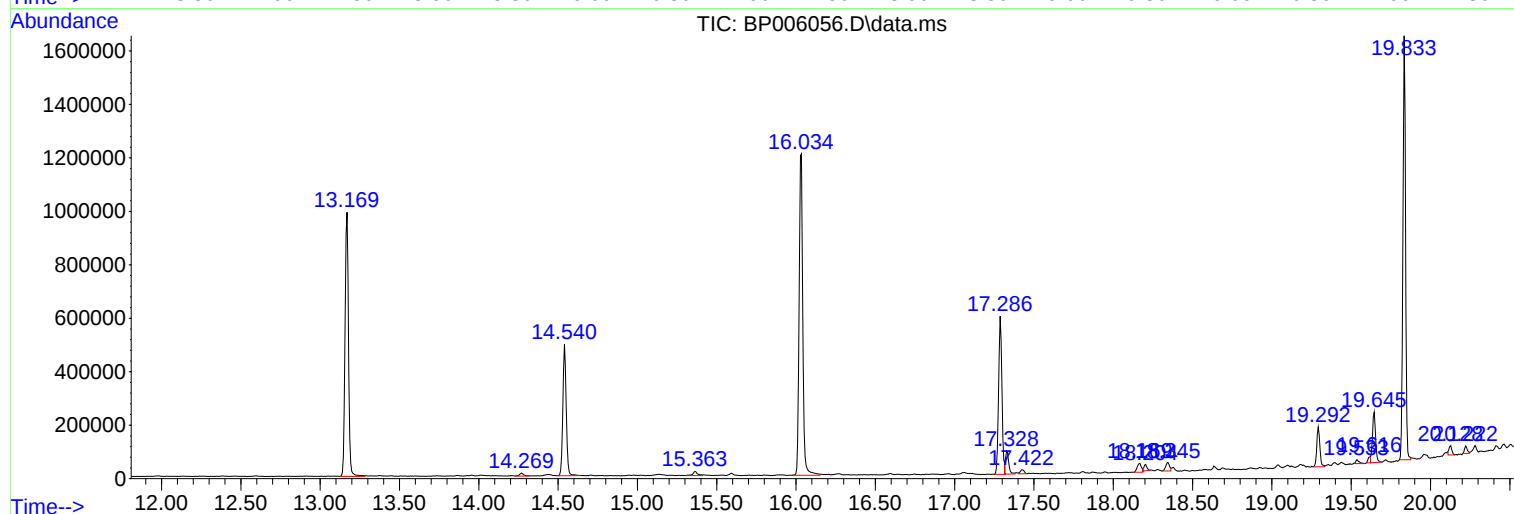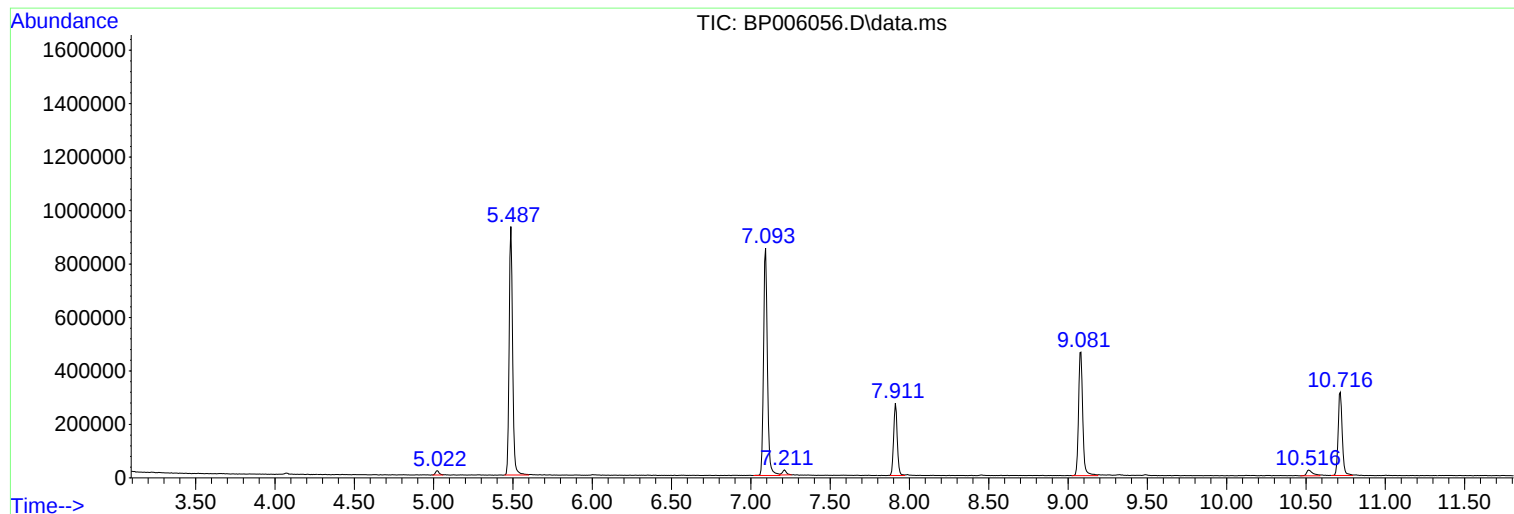

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
Data File : BP006056.D
Acq On : 24 Jun 2021 16:55
Operator : CG/JU
Sample : M2776-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
0339-DISCRETE-CORE-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 3,3-Dimethylbutane-2-ol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.516	2.12 ng	59220	Naphthalene-d8	10.716

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3,3-Dimethylbutane-2-ol	102	C6H14O	000464-07-3	64
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	64
3			Ethanol, 2-[2-(2-butoxyethoxy)et...	206	C10H22O4	000143-22-6	64
4			Propanoic acid, 3-methoxy-, meth...	118	C5H10O3	003852-09-3	64
5			1-Methoxybenzene, -4-(4-iodobenzy...	337	C14H12INO	300686-57-1	59

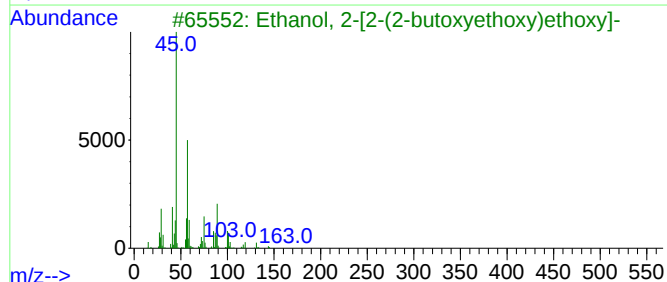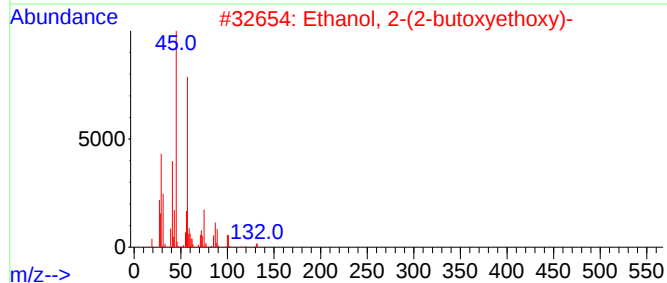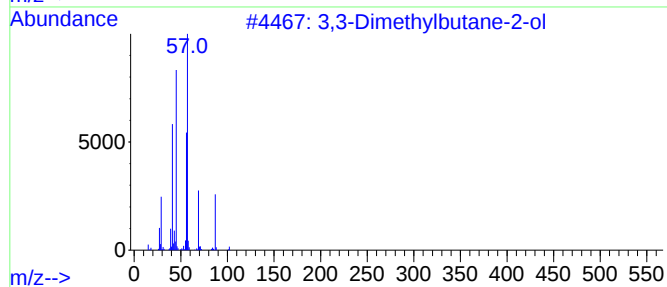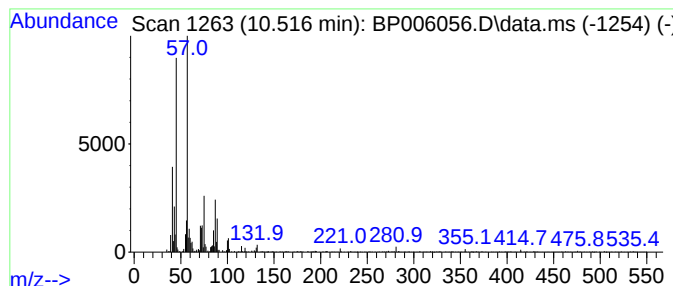

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
Data File : BP006056.D
Acq On : 24 Jun 2021 16:55
Operator : CG/JU
Sample : M2776-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
0339-DISCRETE-CORE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
3,3-Dimethylbut...	10.516	2.1	ng	59220	2	10.716	558098	20.0