

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
 Data File : BP006067.D
 Acq On : 24 Jun 2021 23:08
 Operator : CG/JU
 Sample : M2810-01 2X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 NB-08-062221

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	401	408	420	rBV	295906	476186	37.03%	5.355%
2	7.093	675	681	696	rBV	255184	468866	36.46%	5.273%
3	7.910	813	820	837	rBV	294050	479154	37.26%	5.389%
4	9.081	1012	1019	1039	rBV	154972	298467	23.21%	3.357%
5	10.716	1287	1297	1307	rBV	364007	632749	49.21%	7.116%
6	13.169	1707	1714	1727	rBV	460946	690395	53.69%	7.765%
7	13.863	1827	1832	1840	rBV10	11906	24361	1.89%	0.274%
8	14.434	1922	1929	1935	rBV9	8145	19083	1.48%	0.215%
9	14.539	1938	1947	1956	rBV	534616	823498	64.04%	9.262%
10	14.857	1996	2001	2007	rBV	15926	25976	2.02%	0.292%
11	16.033	2194	2201	2215	rBV	387891	608260	47.30%	6.841%
12	17.286	2408	2414	2420	rBV	632135	947068	73.65%	10.651%
13	17.951	2523	2527	2531	rBV	35560	40754	3.17%	0.458%
14	19.075	2716	2718	2724	rVB6	46426	51819	4.03%	0.583%
15	19.833	2843	2847	2853	rVB	852447	1009070	78.47%	11.349%
16	21.363	3103	3107	3118	rVB	921178	1285890	100.00%	14.462%
17	23.768	3512	3516	3523	rVB2	544017	1009972	78.54%	11.359%




Sum of corrected areas: 8891568

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
Data File : BP006067.D
Acq On : 24 Jun 2021 23:08
Operator : CG/JU
Sample : M2810-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
NB-08-062221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

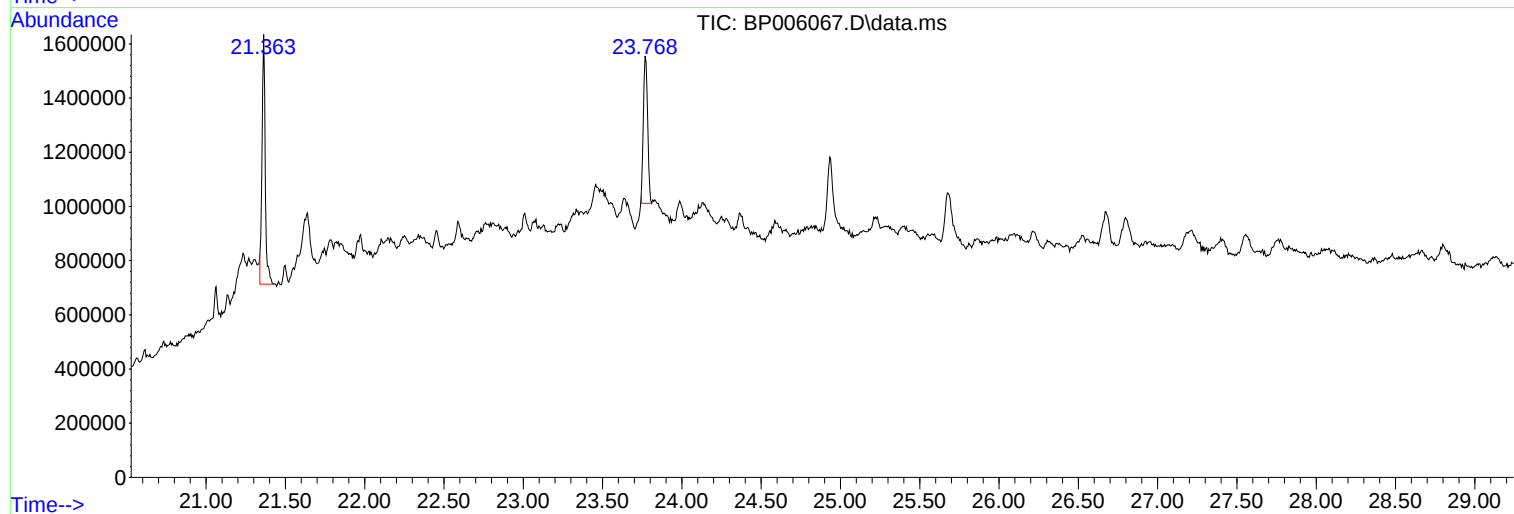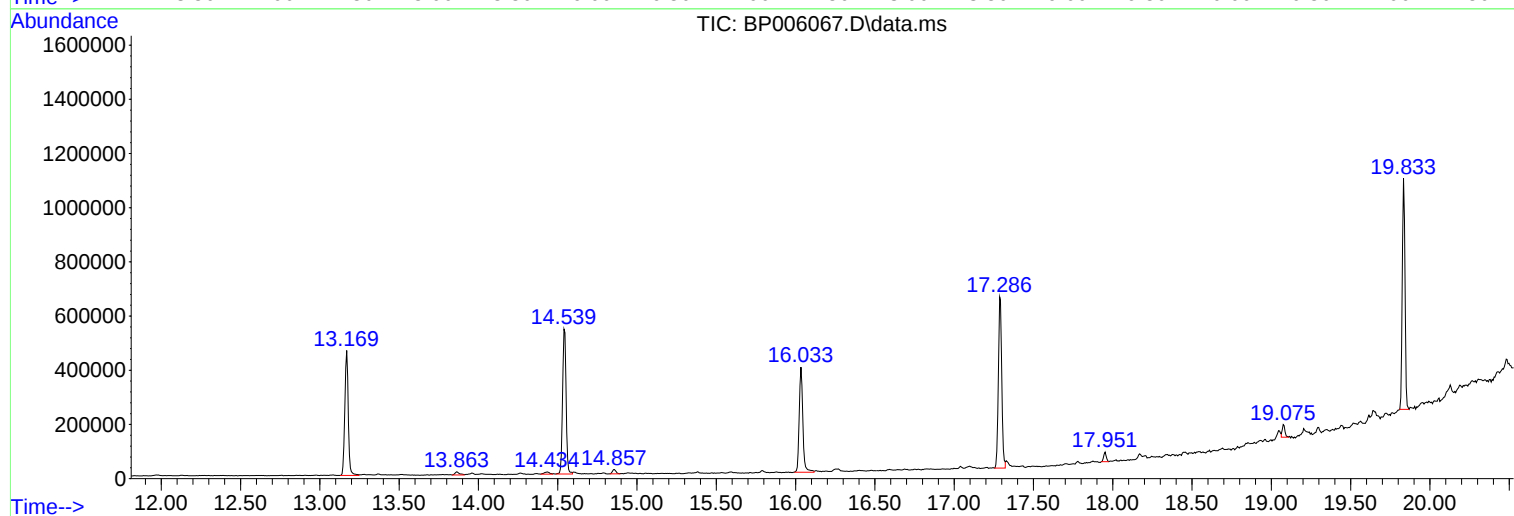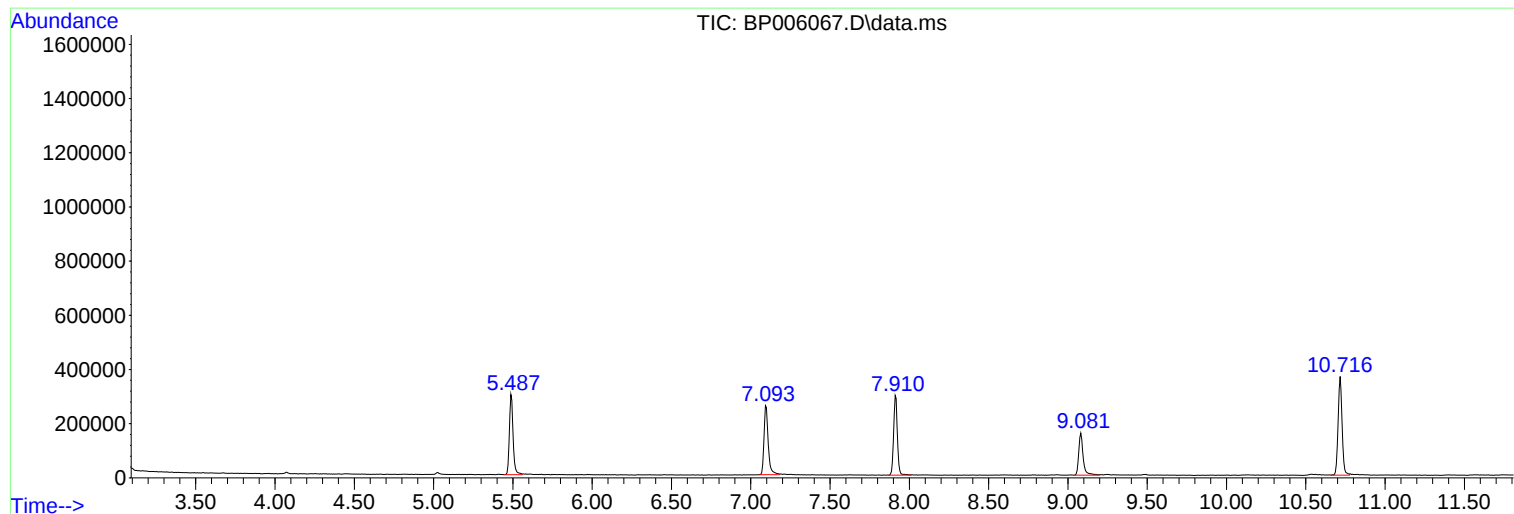

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
Data File : BP006067.D
Acq On : 24 Jun 2021 23:08
Operator : CG/JU
Sample : M2810-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
NB-08-062221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
Data File : BP006067.D
Acq On : 24 Jun 2021 23:08
Operator : CG/JU
Sample : M2810-01 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
NB-08-062221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------