


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
 Data File : BP006047.D
 Acq On : 24 Jun 2021 11:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 22 17:52:38 2021

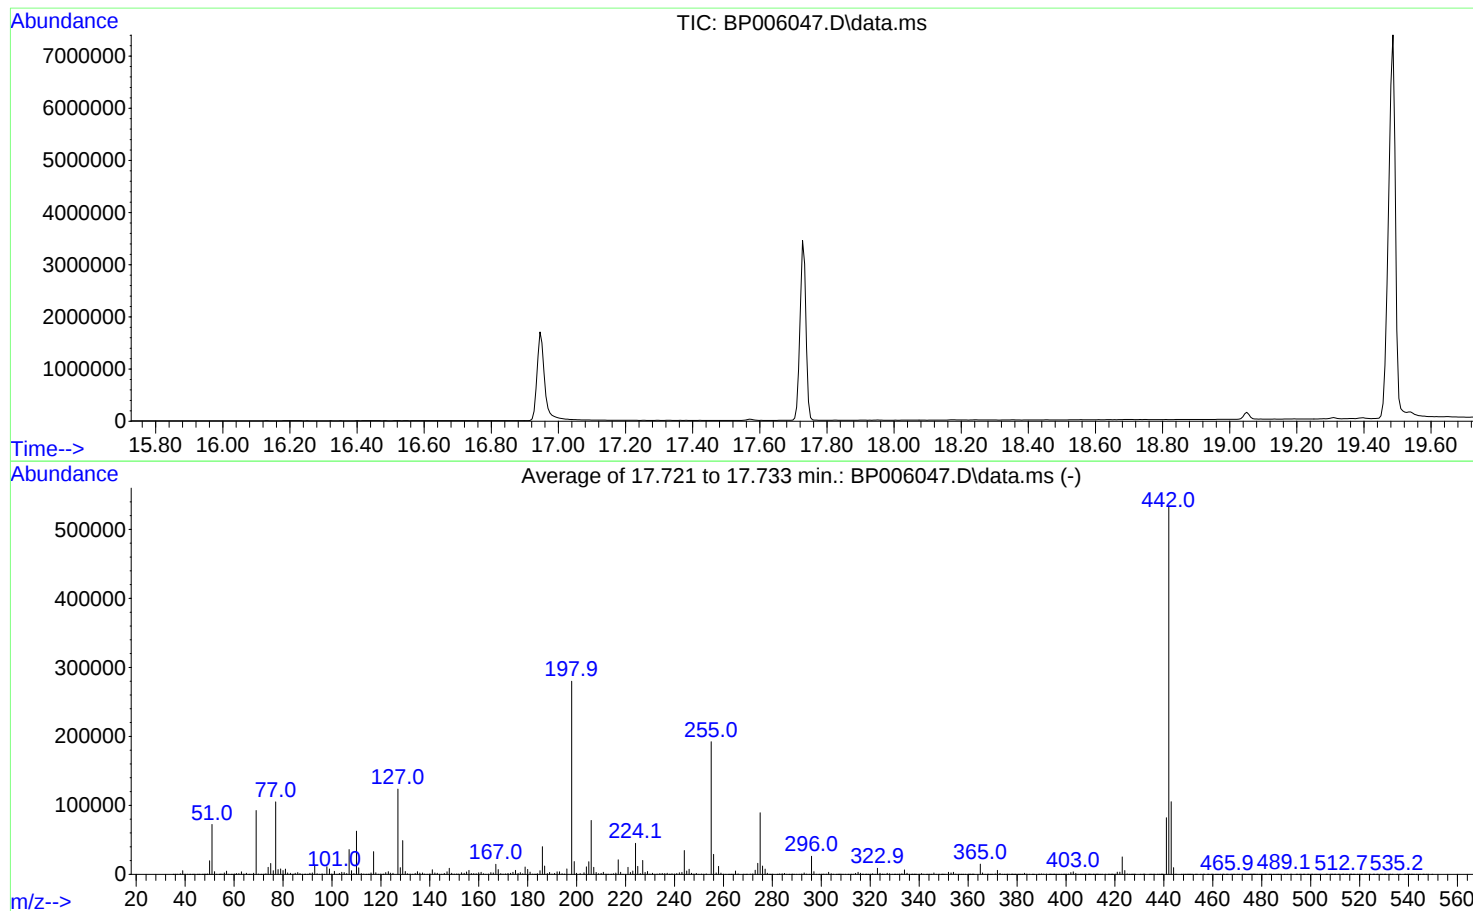




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	72363	PASS
68	69	0.00	2	1.9	1740	PASS
69	198	0.00	100	33.1	92647	PASS
70	69	0.00	2	0.4	413	PASS
127	198	10	80	44.1	123603	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	280019	PASS
199	198	5	9	6.6	18602	PASS
275	198	10	60	31.9	89376	PASS
365	198	1	100	5.3	14778	PASS
441	198	0.01	100	29.3	82176	PASS
442	442	100	100	100.0	533227	PASS
443	442	15	24	19.8	105319	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
 Data File : BP006047.D
 Acq On : 24 Jun 2021 11:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 24 12:40:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 22 17:52:38 2021
 Response via : Initial Calibration

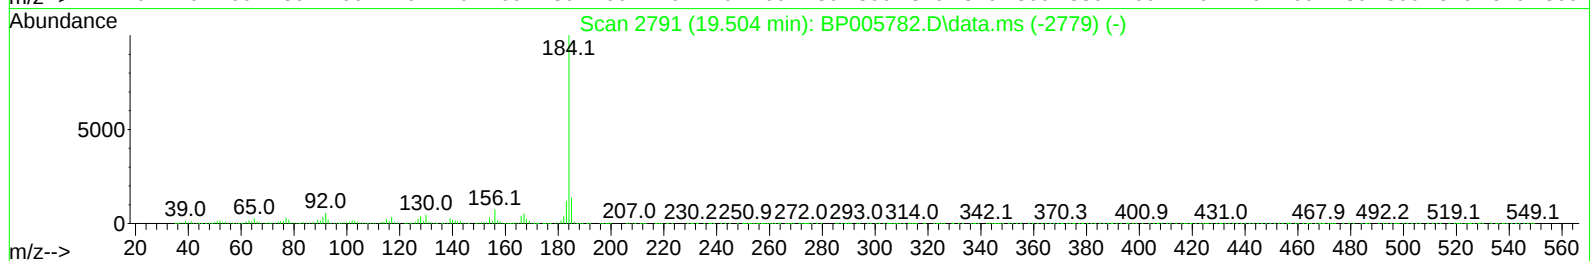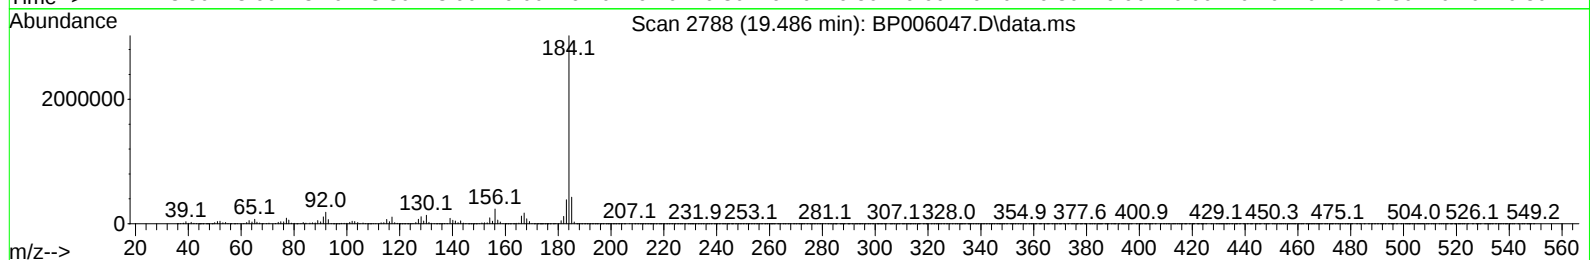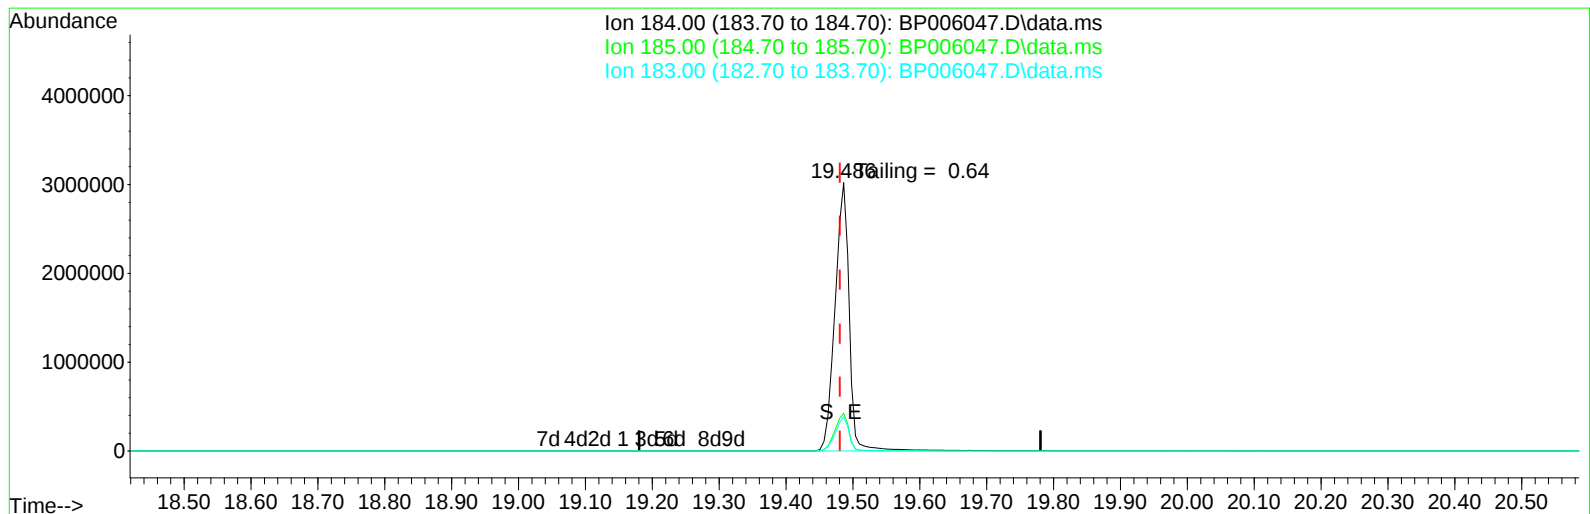

TIC: BP006047.D\data.ms

(77) Benzidine

19.486min (+ 0.006) 4335076.85 ng m




response 4420010

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.09
183.00	11.90	12.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062421\
 Data File : BP006047.D
 Acq On : 24 Jun 2021 11:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 24 12:40:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 22 17:52:38 2021
 Response via : Initial Calibration

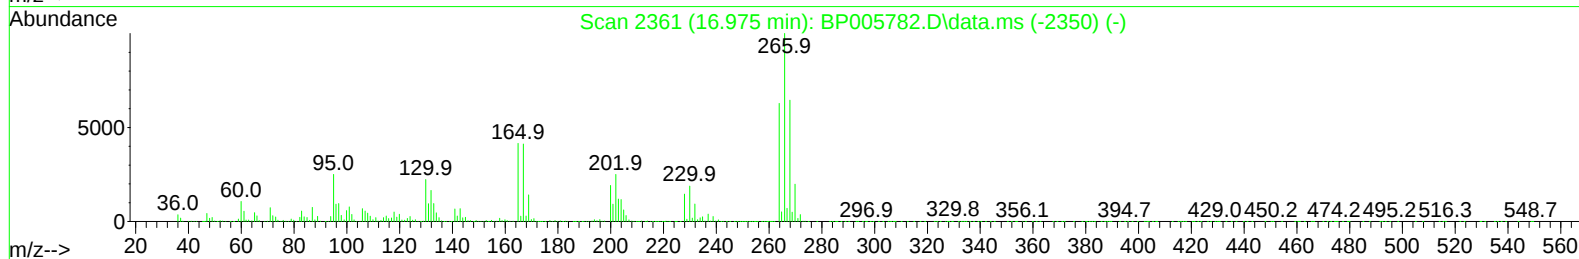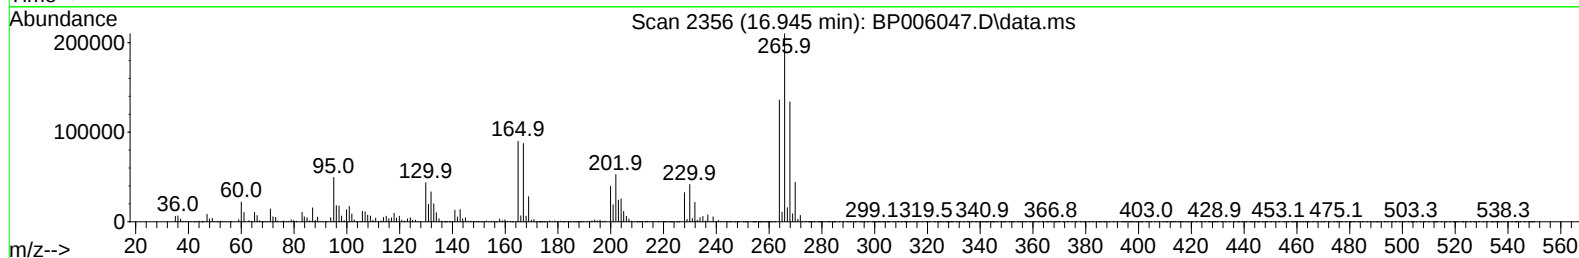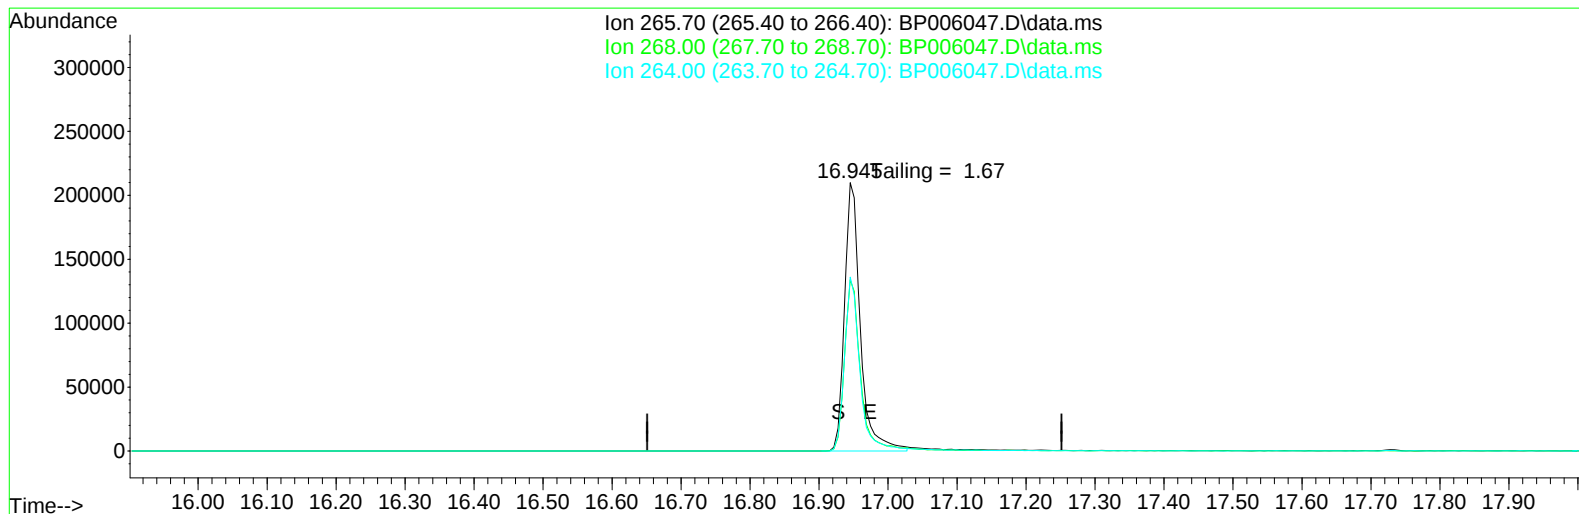

TIC: BP006047.D\data.ms

(70) Pentachlorophenol (C)

16.945min (-0.006) 2209941.37 ng m

response 340285

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.78
264.00	62.90	64.79
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
6/24/2021	BNA_P	BP006047.D
Compound Name	Response	Retention Time
DDT	1066797	20.66
DDD	19441	20.23
DDE	2690	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22131	1088928	2.03

Instrument :
BNA_P
ClientSampleId :
DFTPP