

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010796.D
 Acq On : 24 Jun 2022 16:42
 Operator : CG/JU
 Sample : N3396-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0168

Quant Time: Jun 24 22:46:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 22:42:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	420345	20.000	ng/ul	0.00
20) Naphthalene-d8	10.516	136	1712252	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.375	164	911518	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	1616247	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.251	240	1325493	20.000	ng/ul	# 0.00
88) Perylene-d12	23.621	264	1486548	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	54862	4.937	ng/uL	0.00
4) Pyridine-d5	3.611	84	314471	10.632	ng/ul	0.00
7) Phenol-d5	6.887	99	250104	7.516	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	723711	33.257	ng/ul	0.00
11) 2-Chlorophenol-d4	7.252	132	716376	25.949	ng/ul	0.00
15) 4-Methylphenol-d8	8.428	113	458872	17.445	ng/ul	0.00
21) Nitrobenzene-d5	8.881	128	404800	37.137	ng/ul	0.00
24) 2-Nitrophenol-d4	9.604	143	338226	37.506	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.134	165	663902	29.795	ng/ul	0.00
31) 4-Chloroaniline-d4	10.657	131	1091473	30.008	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	2187655	35.036	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	2719578	34.127	ng/ul	0.00
54) 4-Nitrophenol-d4	14.575	143	49952	5.122	ng/ul	0.00
60) Fluorene-d10	15.375	176	1854426	34.609	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	128846	24.062	ng/ul	0.00
73) Anthracene-d10	17.239	188	2636145	36.659	ng/ul	0.00
81) Pyrene-d10	19.492	212	2709390	37.519	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.468	264	2752700	37.473	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.546	105	47265	1.170	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010796.D
Acq On : 24 Jun 2022 16:42
Operator : CG/JU
Sample : N3396-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0168

Quant Time: Jun 24 22:46:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 22:42:26 2022
Response via : Initial Calibration

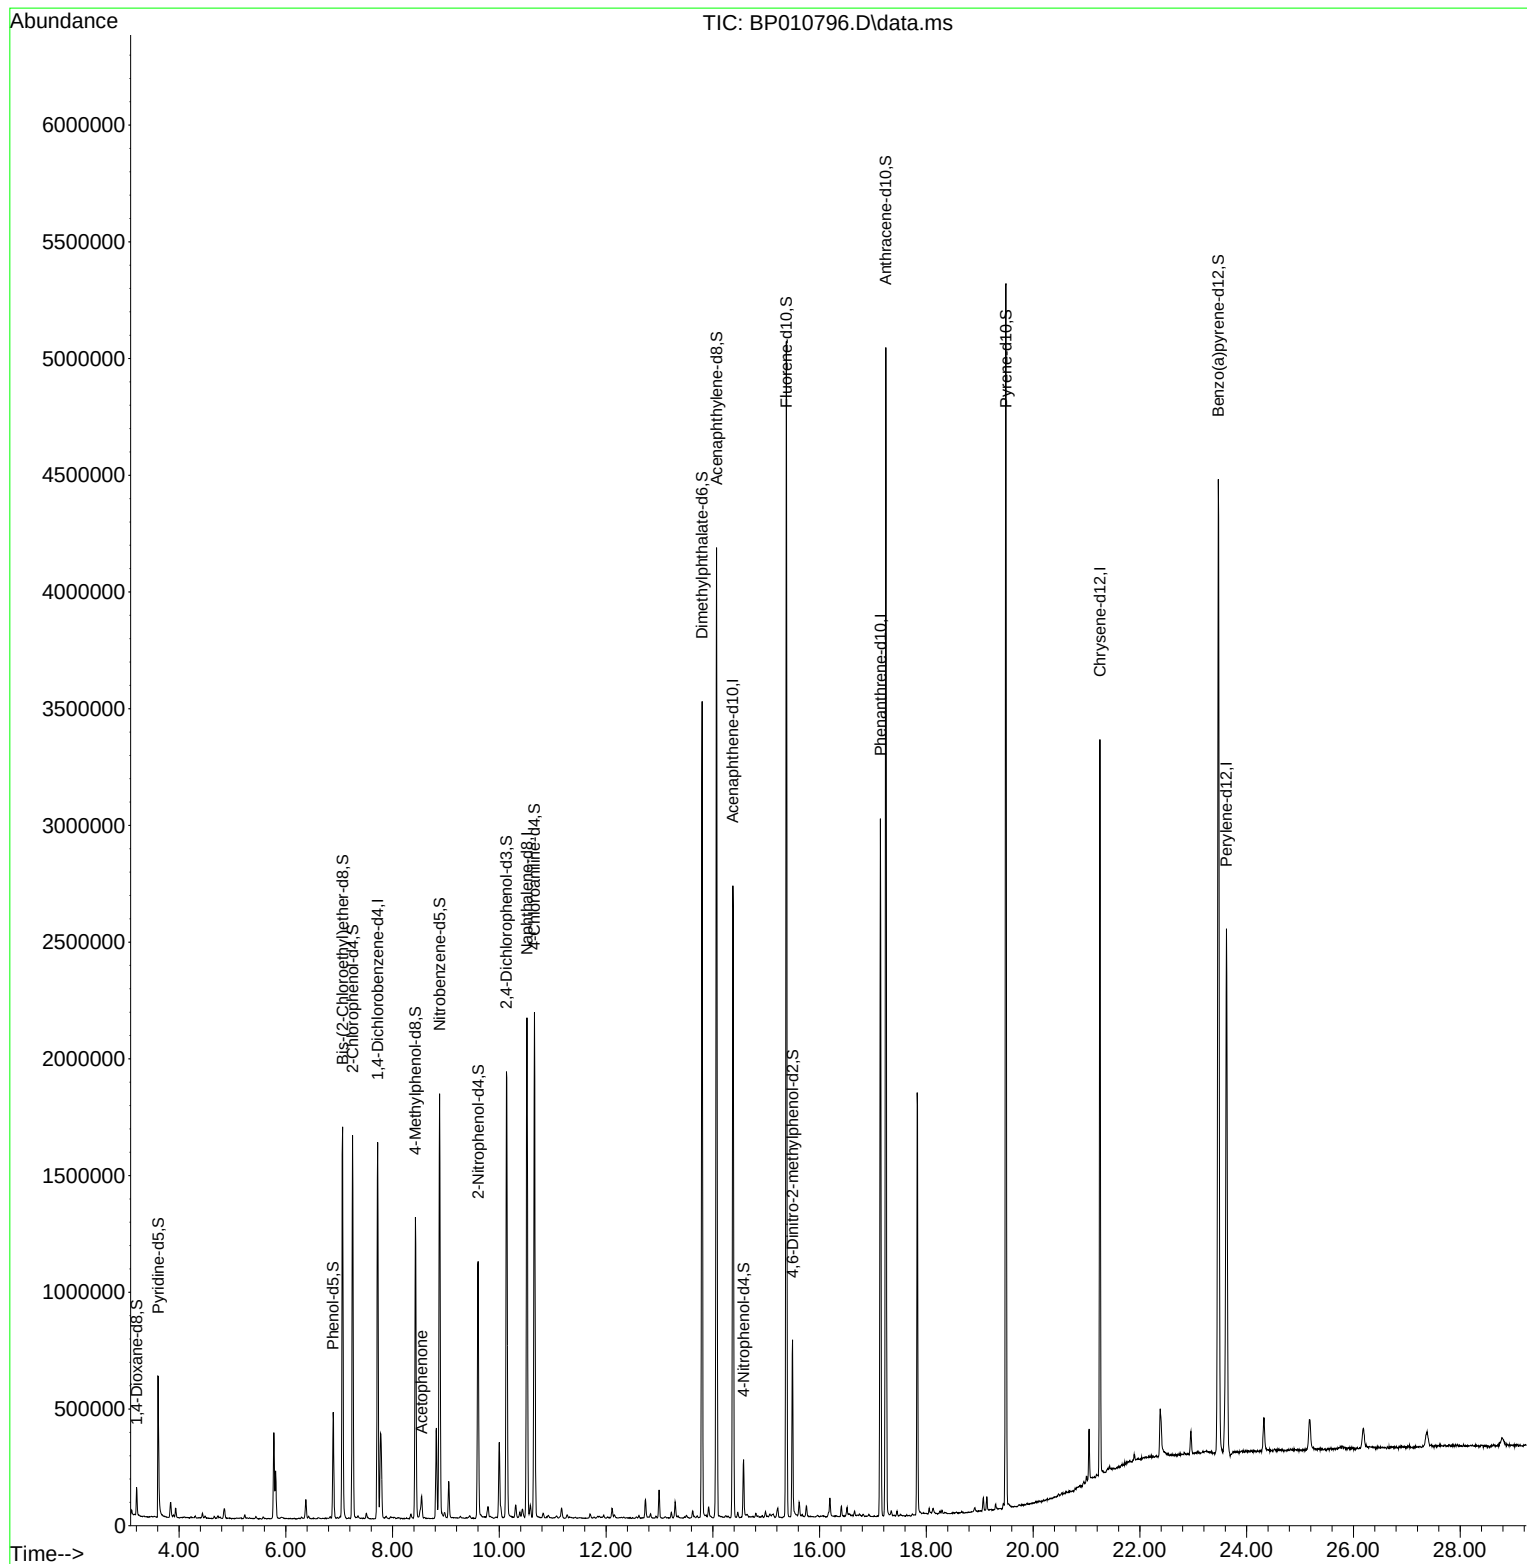

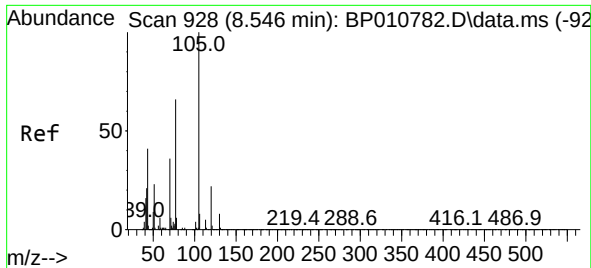

#16
 Acetophenone
 Concen: 1.170 ng/ul
 RT: 8.546 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BP010796.D
 Acq: 24 Jun 2022 16:42

Instrument :
 BNA_P
 ClientSampleId :
 C0168

Tgt Ion:105 Resp: 47265
 Ion Ratio Lower Upper
 105 100
 77 78.6 67.5 101.3
 51 27.5 29.6 44.4#

