

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010795.D
 Acq On : 24 Jun 2022 16:08
 Operator : CG/JU
 Sample : N3396-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0167

Quant Time: Jun 24 22:46:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 22:42:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	391079	20.000	ng/ul	0.00
20) Naphthalene-d8	10.516	136	1570047	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.375	164	835894	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.140	188	1555854	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.251	240	1432289	20.000	ng/ul	# 0.00
88) Perylene-d12	23.622	264	1581835	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	50169	4.853	ng/uL	0.00
4) Pyridine-d5	3.611	84	135972	4.941	ng/ul	0.00
7) Phenol-d5	6.887	99	184142	5.948	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.064	67	649842	32.097	ng/ul	0.00
11) 2-Chlorophenol-d4	7.252	132	597541	23.264	ng/ul	0.00
15) 4-Methylphenol-d8	8.428	113	352326	14.397	ng/ul	0.00
21) Nitrobenzene-d5	8.881	128	358885	35.907	ng/ul	0.00
24) 2-Nitrophenol-d4	9.599	143	274009	33.137	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.134	165	557123	27.268	ng/ul	0.00
31) 4-Chloroaniline-d4	10.657	131	904648	27.125	ng/ul	0.00
46) Dimethylphthalate-d6	13.799	166	1935180	33.797	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	2391370	32.723	ng/ul	0.00
54) 4-Nitrophenol-d4	14.569	143	33170	3.709	ng/ul	-0.01
60) Fluorene-d10	15.375	176	1653547	33.652	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.493	200	84558	16.404	ng/ul	0.00
73) Anthracene-d10	17.240	188	2453861	35.449	ng/ul	0.00
81) Pyrene-d10	19.492	212	2676790	34.304	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.469	264	2827373	36.171	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.546	105	37918	1.009	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010795.D
Acq On : 24 Jun 2022 16:08
Operator : CG/JU
Sample : N3396-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0167


Quant Time: Jun 24 22:46:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 22:42:26 2022
Response via : Initial Calibration

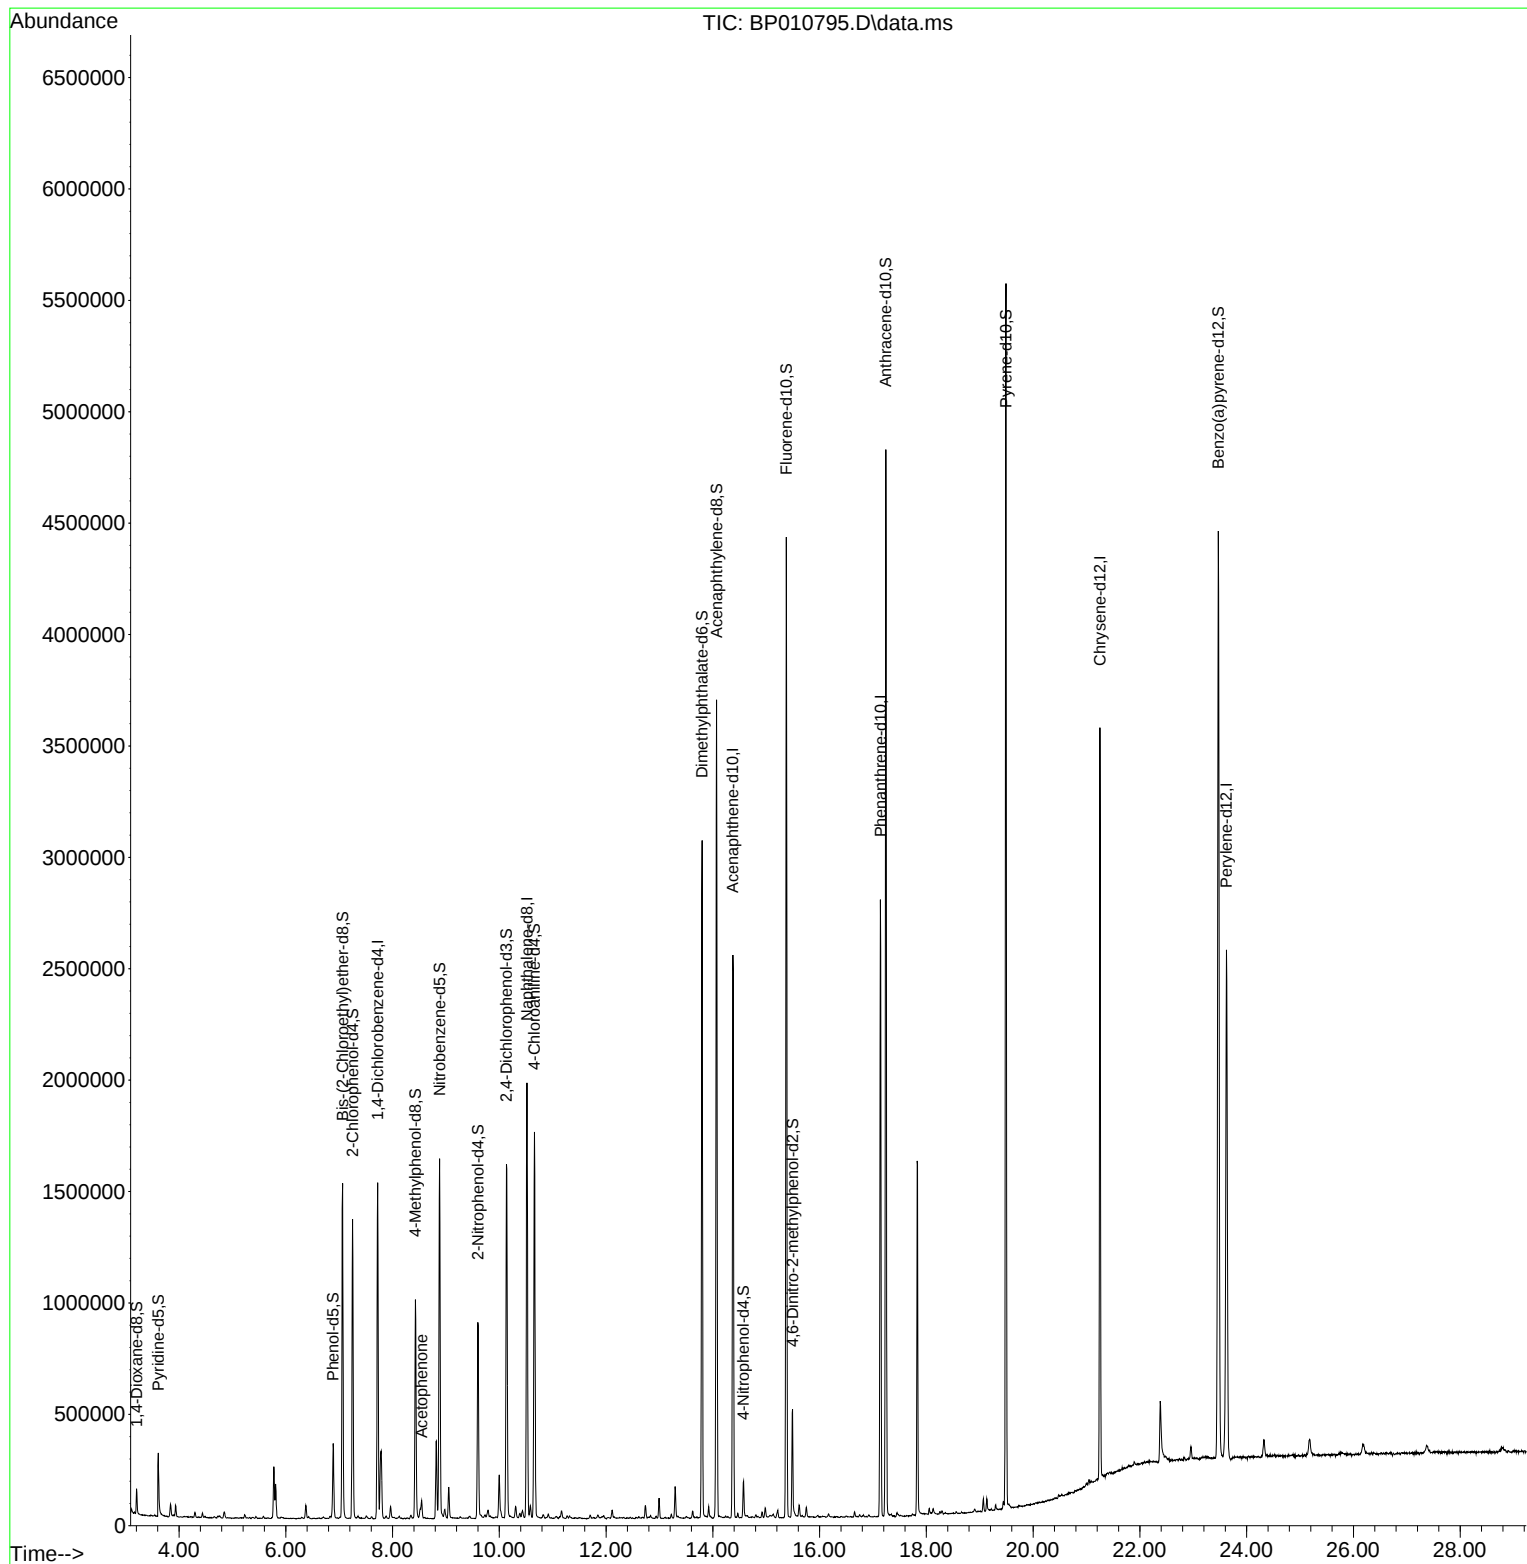

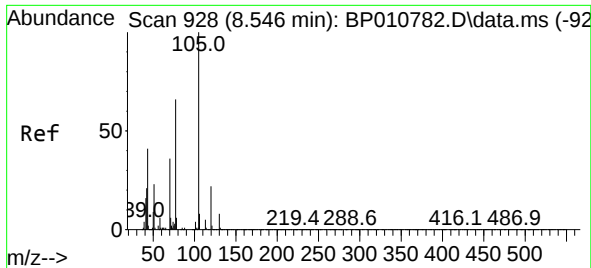

#16
 Acetophenone
 Concen: 1.009 ng/ul
 RT: 8.546 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BP010795.D
 Acq: 24 Jun 2022 16:08

Instrument :
 BNA_P
 ClientSampleId :
 C0167

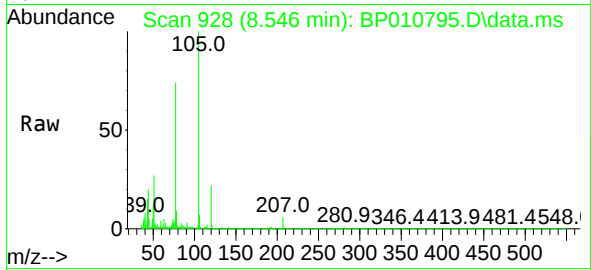

Tgt Ion:105 Resp: 37918
 Ion Ratio Lower Upper
 105 100
 77 73.9 67.5 101.3
 51 26.6 29.6 44.4#

