

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010806.D
 Acq On : 24 Jun 2022 22:21
 Operator : CG/JU
 Sample : N3401-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF2

Quant Time: Jun 24 23:41:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 22:42:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	365051	20.000	ng/ul	0.00
20) Naphthalene-d8	10.516	136	1447029	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.375	164	782838	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	1404759	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.251	240	1314120	20.000	ng/ul	# 0.00
88) Perylene-d12	23.621	264	1438535	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	52014	5.390	ng/uL	0.00
4) Pyridine-d5	3.605	84	333047	12.965	ng/ul	0.00
7) Phenol-d5	6.887	99	234680	8.121	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.064	67	673168	35.620	ng/ul	0.00
11) 2-Chlorophenol-d4	7.252	132	694572	28.970	ng/ul	0.00
15) 4-Methylphenol-d8	8.428	113	440220	19.271	ng/ul	0.00
21) Nitrobenzene-d5	8.881	128	404188	43.877	ng/ul	0.00
24) 2-Nitrophenol-d4	9.599	143	338569	44.425	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.134	165	662788	35.197	ng/ul	0.00
31) 4-Chloroaniline-d4	10.657	131	771484	25.098	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	2171801	40.500	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	2685476	39.238	ng/ul	0.00
54) 4-Nitrophenol-d4	14.575	143	67689	8.081	ng/ul	0.00
60) Fluorene-d10	15.375	176	1853172	40.270	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	166015	35.671	ng/ul	0.00
73) Anthracene-d10	17.239	188	2614320	41.829	ng/ul	0.00
81) Pyrene-d10	19.486	212	2872540	40.123	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.469	264	3077398	43.291	ng/ul	0.00
Target Compounds						Qvalue
30) Naphthalene	10.569	128	8495191	112.642	ng/ul	98
36) 2-Methylnaphthalene	12.187	142	102323	2.095	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010806.D
Acq On : 24 Jun 2022 22:21
Operator : CG/JU
Sample : N3401-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF2

Quant Time: Jun 24 23:41:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 22:42:26 2022
Response via : Initial Calibration




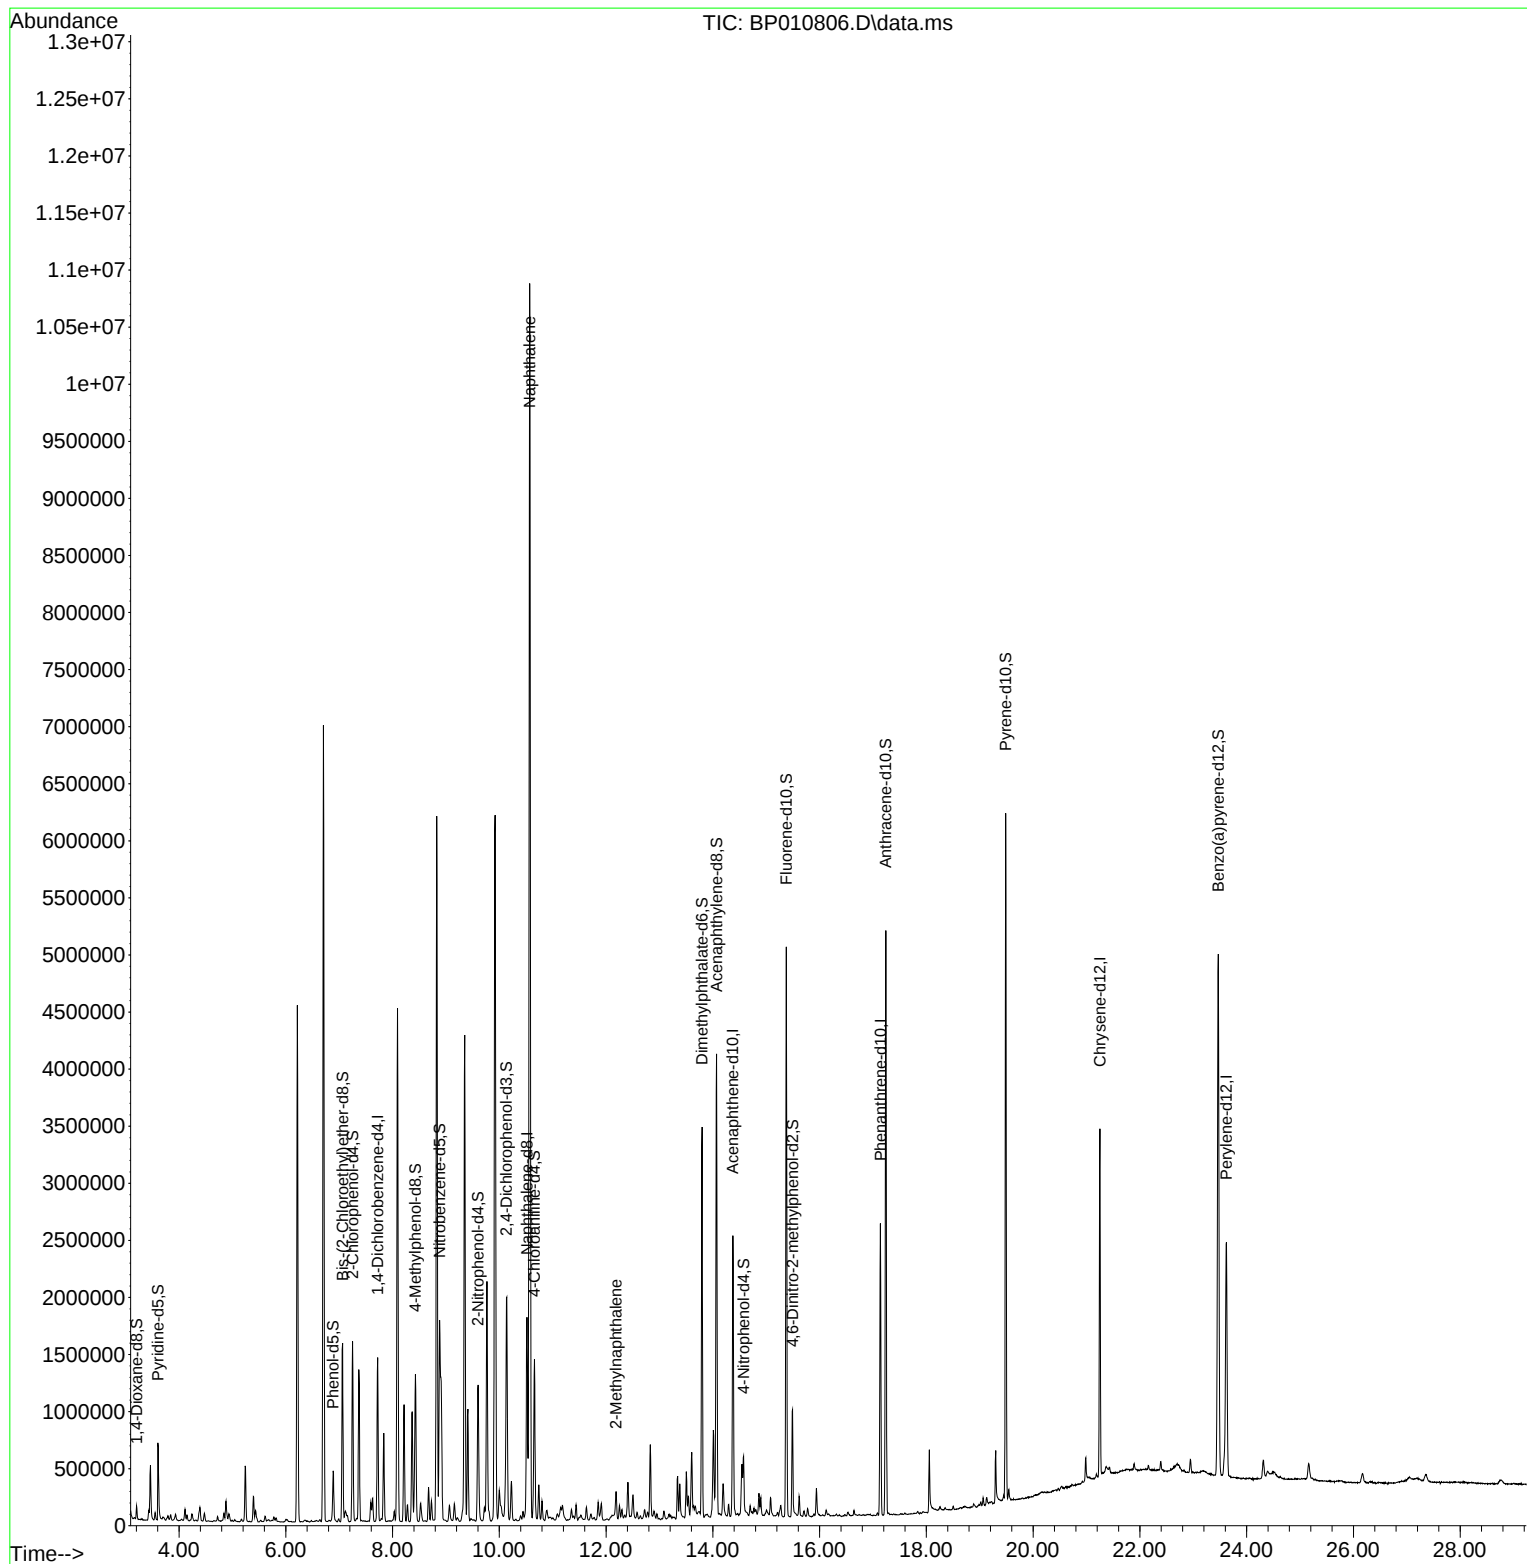


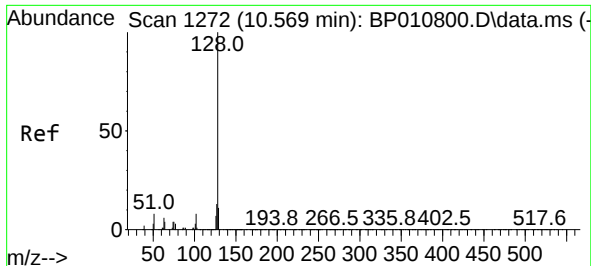

#30
Naphthalene
Concen: 112.642 ng/ul
RT: 10.569 min Scan# 1272
Delta R.T. 0.000 min
Lab File: BP010806.D
Acq: 24 Jun 2022 22:21

Instrument :
BNA_P
ClientSampleId :
C0AF2

Tgt Ion:128 Resp: 8495191
Ion Ratio Lower Upper
128 100
129 11.5 8.7 13.1
127 13.4 10.2 15.4

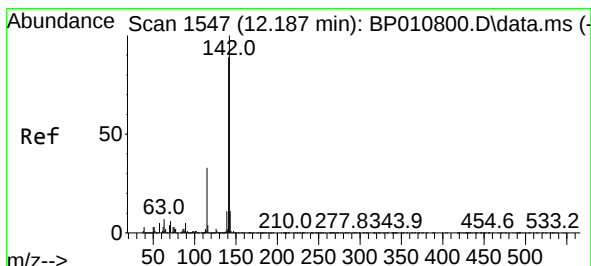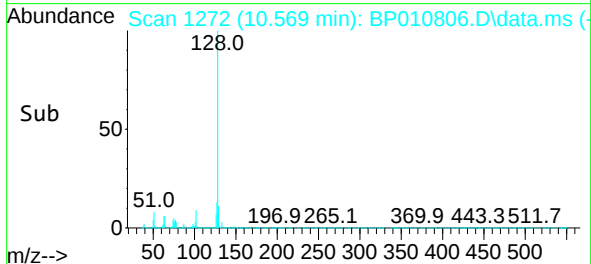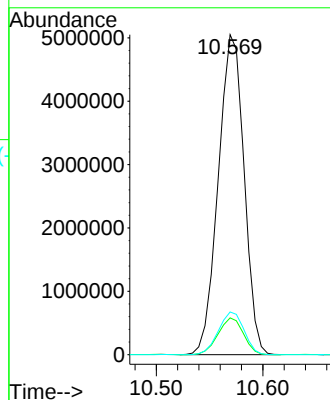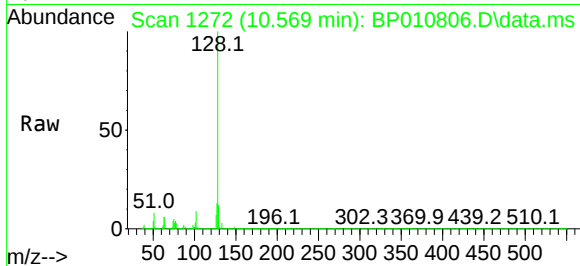

#36
2-Methylnaphthalene
Concen: 2.095 ng/ul
RT: 12.187 min Scan# 1547
Delta R.T. -0.006 min
Lab File: BP010806.D
Acq: 24 Jun 2022 22:21

Tgt Ion:142 Resp: 102323
Ion Ratio Lower Upper
142 100
141 88.5 70.1 105.1

