

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010813.D
 Acq On : 25 Jun 2022 02:18
 Operator : CG/JU
 Sample : N3374-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4T6

Quant Time: Jun 25 03:05:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 22:42:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	382986	20.000	ng/u1	0.00
20) Naphthalene-d8	10.516	136	1490823	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.375	164	781170	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.139	188	1488593	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.251	240	1546829	20.000	ng/u1	# 0.00
88) Perylene-d12	23.627	264	1707993	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	44813	4.426	ng/uL	0.00
4) Pyridine-d5	3.616	84	230115	8.539	ng/u1	0.01
7) Phenol-d5	6.898	99	281918	9.299	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	571168	28.807	ng/u1	0.00
11) 2-Chlorophenol-d4	7.257	132	593636	23.601	ng/u1	0.00
15) 4-Methylphenol-d8	8.434	113	526430	21.965	ng/u1	0.00
21) Nitrobenzene-d5	8.881	128	368984	38.879	ng/u1	0.00
24) 2-Nitrophenol-d4	9.598	143	313161	39.884	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.139	165	557004	28.711	ng/u1	0.00
31) 4-Chloroaniline-d4	10.663	131	336195	10.616	ng/u1	0.00
46) Dimethylphthalate-d6	13.798	166	1917500	35.834	ng/u1	0.00
49) Acenaphthylene-d8	14.069	160	2361266	34.575	ng/u1	0.00
54) 4-Nitrophenol-d4	14.592	143	44773	5.357	ng/u1	0.01
60) Fluorene-d10	15.374	176	1642216	35.762	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	111949	22.699	ng/u1	0.00
73) Anthracene-d10	17.239	188	2320805	35.042	ng/u1	0.00
81) Pyrene-d10	19.492	212	2818859	33.450	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.474	264	3071303	36.389	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.246	88	11563	1.071	ng/uL#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010813.D
Acq On : 25 Jun 2022 02:18
Operator : CG/JU
Sample : N3374-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4T6


Quant Time: Jun 25 03:05:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 22:42:26 2022
Response via : Initial Calibration

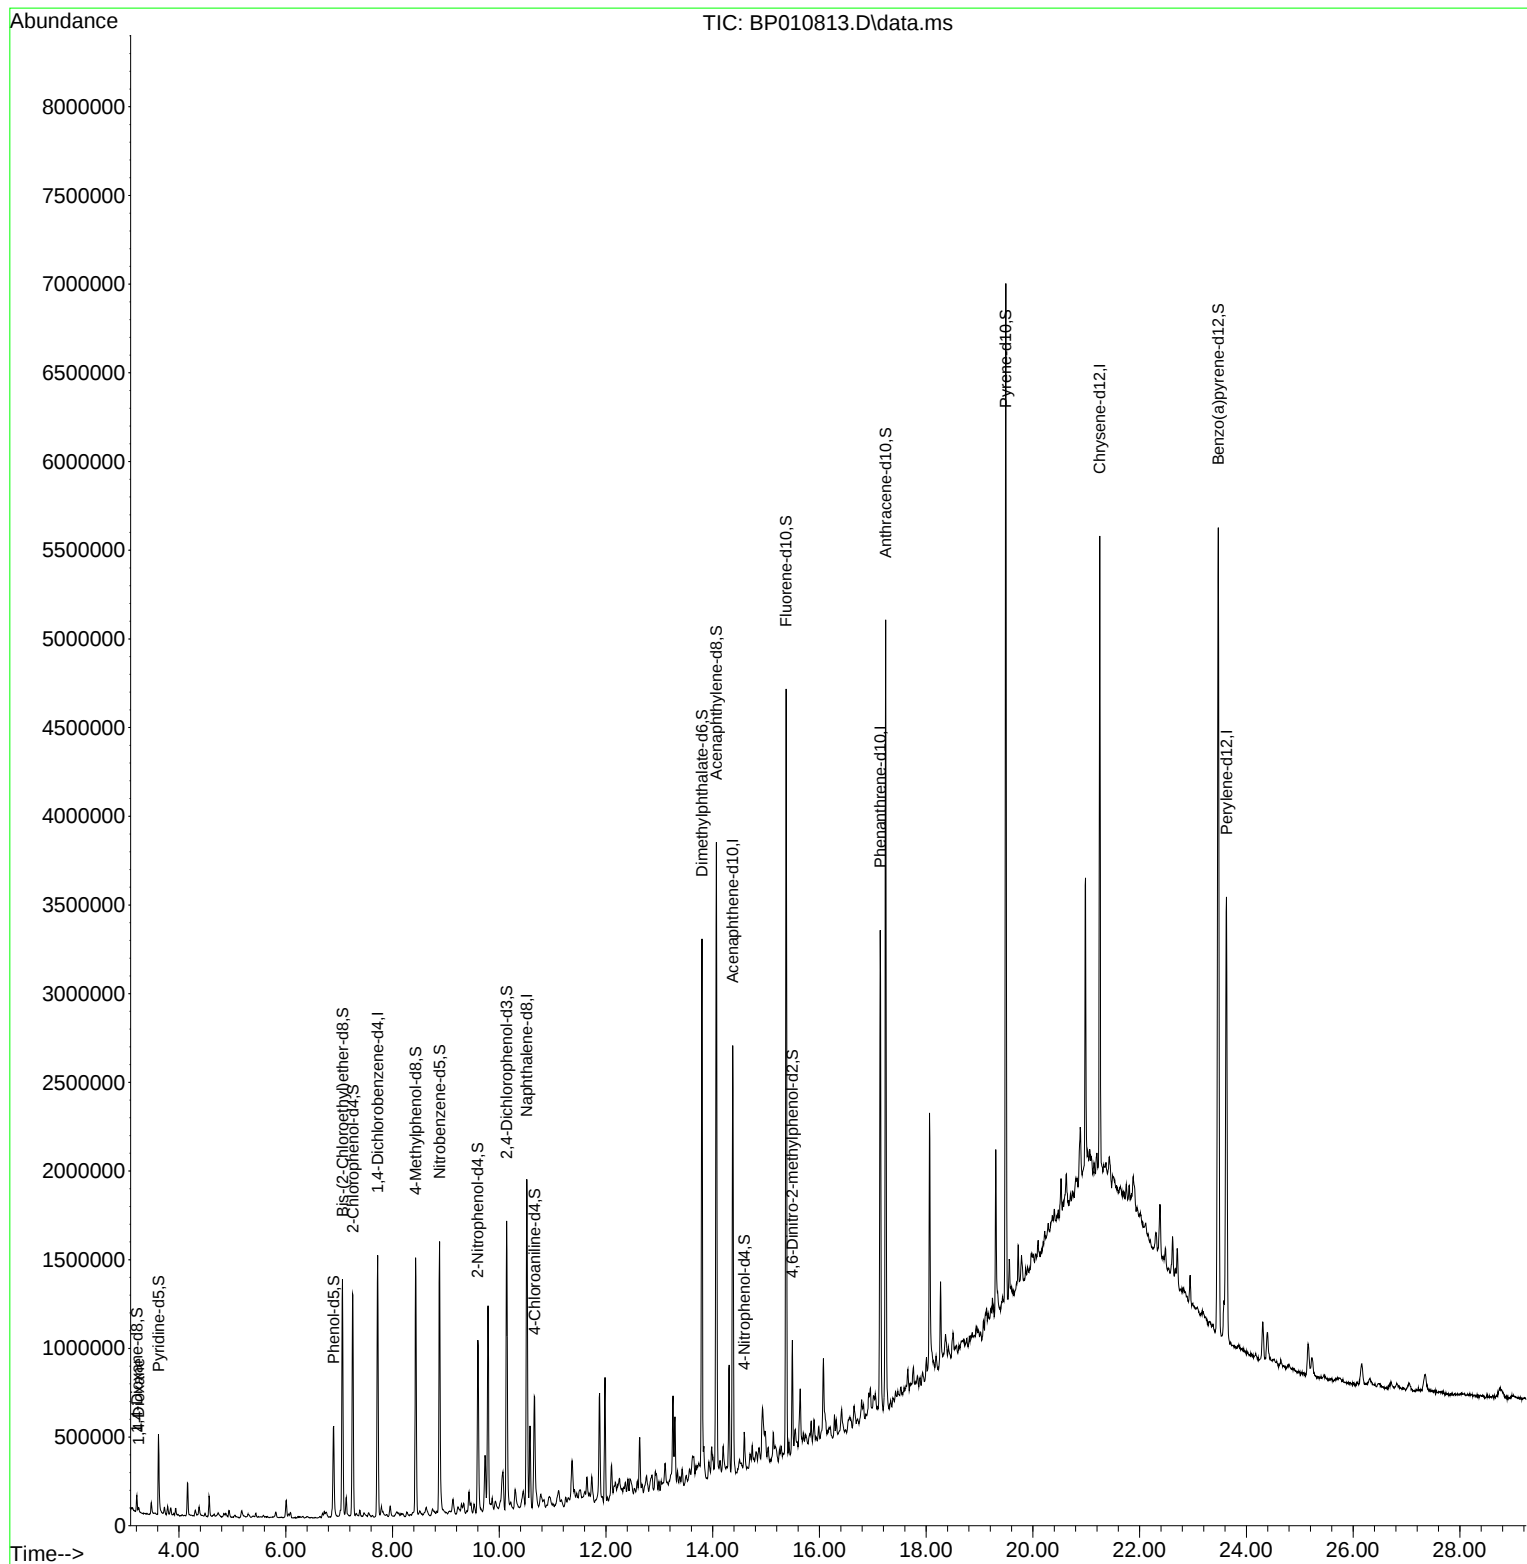

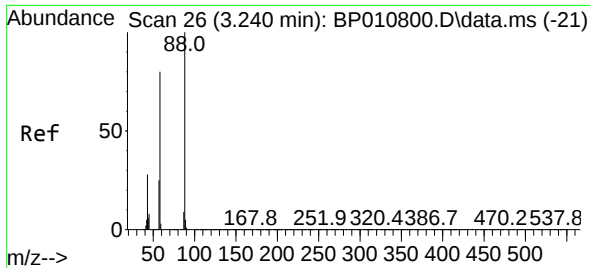

#2
 1,4-Dioxane
 Concen: 1.071 ng/uL
 RT: 3.246 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP010813.D
 Acq: 25 Jun 2022 02:18

Instrument :
 BNA_P
 ClientSampleId :
 EW4T6

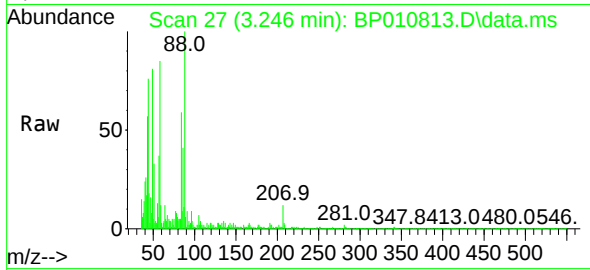

Tgt Ion: 88 Resp: 11563
 Ion Ratio Lower Upper
 88 100
 43 57.5 35.8 53.6#
 58 84.9 68.1 102.1

