

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010784.D
 Acq On : 24 Jun 2022 09:56
 Operator : CG/JU
 Sample : PB145679BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK679

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010784.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	27	rVB	132081	161845	2.38%	0.201%
2	3.605	85	88	111	rBV	1632580	2212772	32.50%	2.746%
3	3.940	140	145	153	rVB	32648	48305	0.71%	0.060%
4	6.887	639	646	655	rBV	1595279	2474515	36.34%	3.071%
5	7.063	669	676	688	rVB	1421889	2107489	30.95%	2.616%
6	7.252	701	708	717	rBV	1684646	2555350	37.53%	3.172%
7	7.722	781	788	797	rVB	1449614	2213745	32.51%	2.748%
8	8.428	901	908	921	rBV	1894233	3029023	44.49%	3.759%
9	8.881	977	985	998	rBV	1437766	2271497	33.36%	2.819%
10	9.605	1096	1108	1120	rBV	861845	1399898	20.56%	1.737%
11	10.140	1189	1199	1212	rBV	1673153	2759054	40.52%	3.424%
12	10.516	1254	1263	1271	rBV	1850531	3123604	45.88%	3.877%
13	10.657	1279	1287	1297	rBV	1942907	3153342	46.31%	3.914%
14	12.116	1528	1535	1543	rBV	36190	63205	0.93%	0.078%
15	13.345	1741	1744	1748	rVB4	6330	6827	0.10%	0.008%
16	13.798	1814	1821	1831	rBV	2905225	3896548	57.23%	4.836%
17	14.069	1859	1867	1875	rBV	3478533	4900729	71.98%	6.083%
18	14.381	1913	1920	1927	rBV	2562084	3730409	54.79%	4.630%
19	14.575	1946	1953	1973	rBV	1112792	1616438	23.74%	2.006%
20	14.804	1990	1992	1998	rVB7	7100	12121	0.18%	0.015%
21	15.381	2083	2090	2100	rBV	4206512	5834998	85.70%	7.242%
22	15.492	2103	2109	2122	rBV	647724	889078	13.06%	1.103%
23	15.616	2126	2130	2135	rVB2	47335	67911	1.00%	0.084%
24	16.163	2221	2223	2229	rVB5	13802	20461	0.30%	0.025%
25	16.816	2331	2334	2341	rVB9	9022	15822	0.23%	0.020%
26	16.922	2349	2352	2356	rBV5	8134	10198	0.15%	0.013%
27	17.145	2383	2390	2397	rBV	2795533	3970577	58.32%	4.928%
28	17.245	2400	2407	2419	rBV	4112906	6005093	88.20%	7.453%
29	18.057	2542	2545	2549	rBV5	11089	14100	0.21%	0.018%
30	19.069	2713	2717	2721	rBV3	49926	68222	1.00%	0.085%
31	19.133	2724	2728	2734	rVV2	48671	64632	0.95%	0.080%
32	19.492	2783	2789	2796	rBV	5170684	6530753	95.92%	8.106%
33	21.257	3084	3089	3108	rVB	3368870	4266885	62.67%	5.296%
34	23.474	3459	3466	3476	rVB2	3601348	6808648	100.00%	8.451%
35	23.627	3485	3492	3502	rVB	2185349	4266666	62.67%	5.296%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010784.D
Acq On : 24 Jun 2022 09:56
Operator : CG/JU
Sample : PB145679BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK679

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 80570760

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010784.D
Acq On : 24 Jun 2022 09:56
Operator : CG/JU
Sample : PB145679BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK679

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

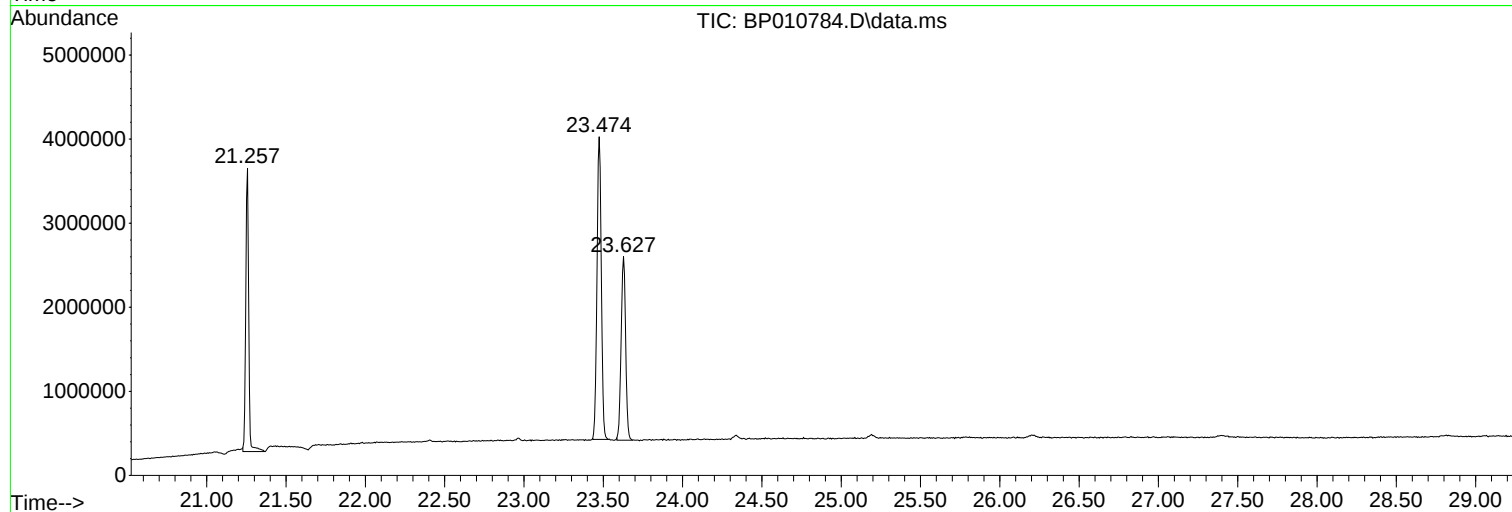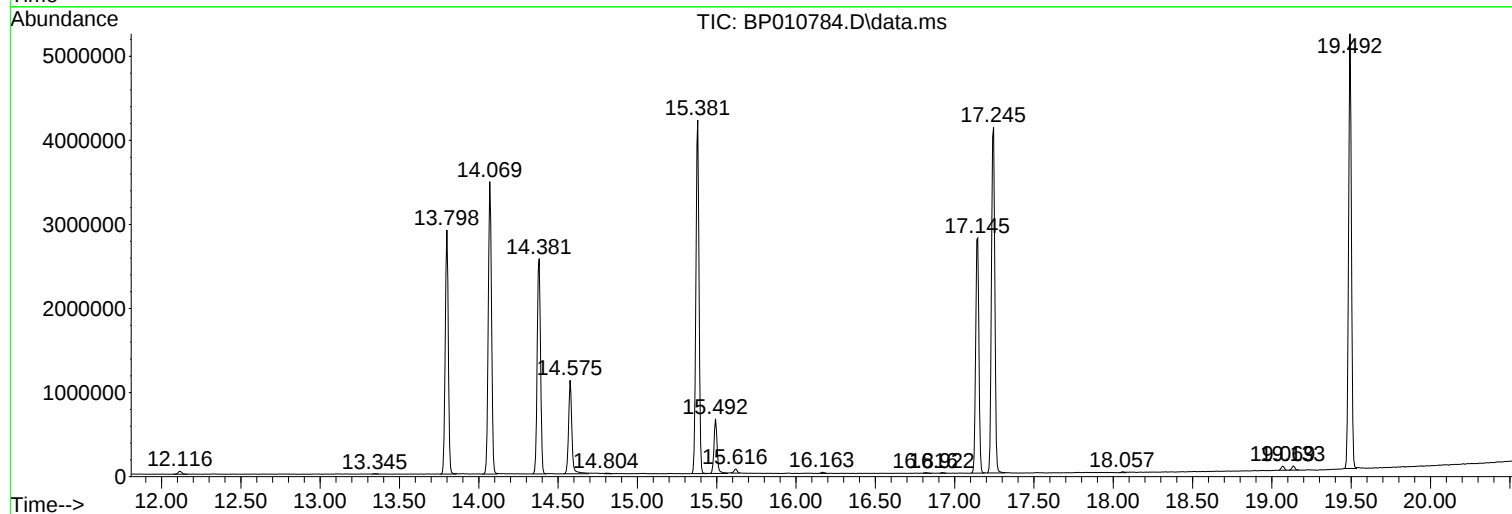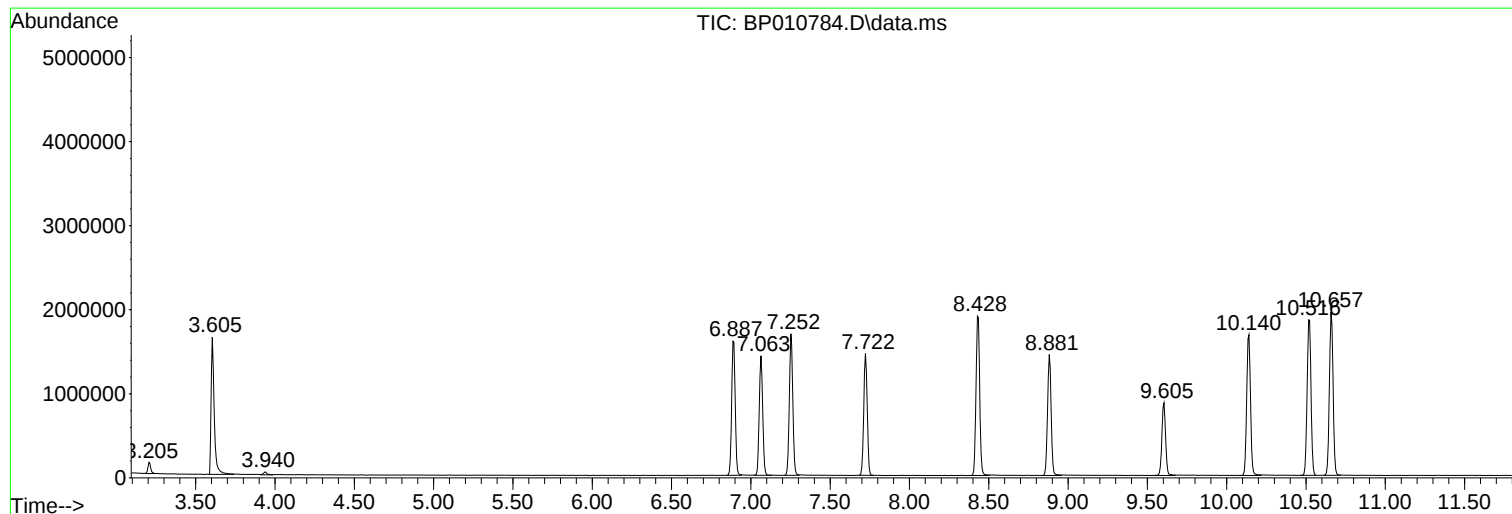

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010784.D
Acq On : 24 Jun 2022 09:56
Operator : CG/JU
Sample : PB145679BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK679

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010784.D
Acq On : 24 Jun 2022 09:56
Operator : CG/JU
Sample : PB145679BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK679

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc