

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010785.D
 Acq On : 24 Jun 2022 10:30
 Operator : CG/JU
 Sample : N3395-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	27	rVB	87670	109622	1.44%	0.169%
2	3.476	63	66	71	rBV	35178	46042	0.61%	0.071%
3	3.605	85	88	107	rBV	502229	743074	9.78%	1.147%
4	3.846	124	129	134	rVV	45710	65766	0.87%	0.102%
5	3.899	134	138	141	rVV6	7277	9684	0.13%	0.015%
6	3.940	141	145	150	rVB	26114	35907	0.47%	0.055%
7	4.223	187	193	197	rBV	26002	37707	0.50%	0.058%
8	4.311	204	208	213	rVB7	6311	10623	0.14%	0.016%
9	4.658	263	267	271	rVB4	5660	8846	0.12%	0.014%
10	4.728	273	279	282	rBV7	9839	12134	0.16%	0.019%
11	4.840	293	298	303	rBV	21174	34082	0.45%	0.053%
12	5.446	395	401	405	rVB3	9566	15741	0.21%	0.024%
13	6.887	640	646	657	rVB	323443	496305	6.53%	0.766%
14	7.064	669	676	684	rBV	1215044	1836641	24.16%	2.836%
15	7.134	684	688	693	rVB	22303	30367	0.40%	0.047%
16	7.252	699	708	718	rBV	1137511	1750577	23.03%	2.703%
17	7.358	723	726	732	rVB6	9521	14623	0.19%	0.023%
18	7.722	781	788	795	rBV	1123101	1699406	22.36%	2.624%
19	7.793	795	800	804	rVB2	12198	20216	0.27%	0.031%
20	8.428	900	908	919	rBV	882655	1357683	17.86%	2.096%
21	8.881	978	985	1000	rBV	1237397	1960036	25.79%	3.026%
22	8.987	1001	1003	1011	rVV9	6866	14535	0.19%	0.022%
23	9.058	1011	1015	1020	rVB9	5275	10497	0.14%	0.016%
24	9.322	1056	1060	1067	rVB3	19107	28370	0.37%	0.044%
25	9.605	1101	1108	1117	rBV	664569	1066048	14.03%	1.646%
26	10.140	1191	1199	1208	rBV	1320534	2144377	28.21%	3.311%
27	10.516	1255	1263	1273	rBV	1400261	2327423	30.62%	3.594%
28	10.658	1279	1287	1298	rBV	1097273	1765707	23.23%	2.726%
29	11.999	1507	1515	1518	rBV8	5688	11905	0.16%	0.018%
30	12.116	1530	1535	1540	rVB2	28295	44982	0.59%	0.069%
31	12.993	1681	1684	1689	rVB5	5766	9460	0.12%	0.015%
32	13.222	1718	1723	1729	rVB3	15505	22869	0.30%	0.035%
33	13.281	1729	1733	1736	rBV6	3924	7696	0.10%	0.012%
34	13.799	1814	1821	1831	rBV	2570961	3434076	45.18%	5.302%
35	14.069	1859	1867	1876	rBV	2968135	4128248	54.31%	6.374%
36	14.381	1912	1920	1928	rBV	1790273	2697028	35.48%	4.164%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010785.D
 Acq On : 24 Jun 2022 10:30
 Operator : CG/JU
 Sample : N3395-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	14.575	1946	1953	1959	rBV	172570	267147	3.51%	0.412%
38	14.804	1990	1992	1999	rVB8	7948	10909	0.14%	0.017%
39	15.134	2044	2048	2055	rVB	44146	62631	0.82%	0.097%
40	15.204	2055	2060	2065	rBV3	8153	14546	0.19%	0.022%
41	15.375	2083	2089	2100	rBV	3823535	5234605	68.87%	8.082%
42	15.493	2103	2109	2116	rBV	409263	582295	7.66%	0.899%
43	15.616	2126	2130	2136	rVB	41395	60500	0.80%	0.093%
44	15.945	2183	2186	2191	rVB4	7289	9804	0.13%	0.015%
45	16.069	2202	2207	2208	rBV5	5093	7801	0.10%	0.012%
46	16.169	2220	2224	2230	rVB7	15367	20948	0.28%	0.032%
47	16.816	2332	2334	2340	rVB7	7390	11206	0.15%	0.017%
48	17.140	2383	2389	2396	rBV	2056522	2910270	38.29%	4.494%
49	17.240	2400	2406	2420	rVV	3981710	5785408	76.12%	8.933%
50	17.340	2420	2423	2429	rVB8	12543	20365	0.27%	0.031%
51	17.775	2495	2497	2503	rVB6	7241	7865	0.10%	0.012%
52	17.845	2503	2509	2513	rVB3	45368	60698	0.80%	0.094%
53	18.057	2541	2545	2552	rBV	66006	97781	1.29%	0.151%
54	19.069	2713	2717	2723	rVB	51738	63931	0.84%	0.099%
55	19.134	2724	2728	2734	rBV	50122	66278	0.87%	0.102%
56	19.298	2753	2756	2761	rBV3	52819	71568	0.94%	0.111%
57	19.492	2783	2789	2795	rBV	5177467	6603816	86.88%	10.197%
58	20.992	3040	3044	3050	rBV	104604	163070	2.15%	0.252%
59	21.251	3083	3088	3097	rBV2	2593250	3228524	42.48%	4.985%
60	21.898	3195	3198	3204	rVB	118104	149702	1.97%	0.231%
61	23.474	3458	3466	3482	rVB	4007084	7600859	100.00%	11.736%
62	23.622	3484	3491	3502	rVB2	1764726	3644028	47.94%	5.627%




Sum of corrected areas: 64764858

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010785.D
Acq On : 24 Jun 2022 10:30
Operator : CG/JU
Sample : N3395-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0158

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

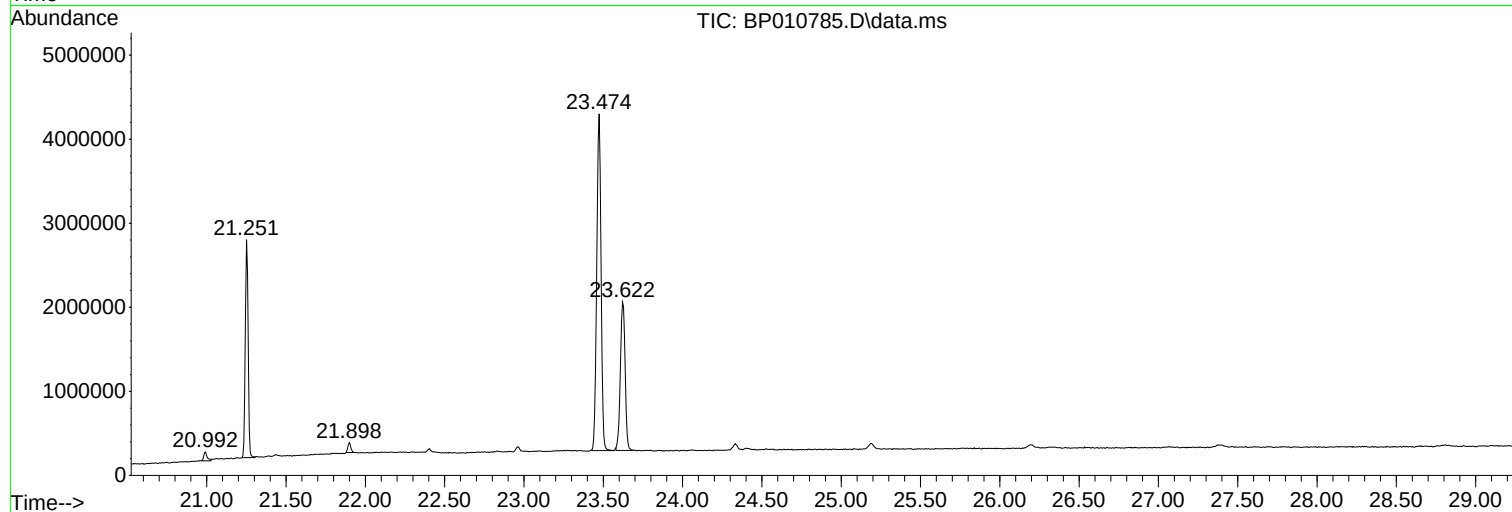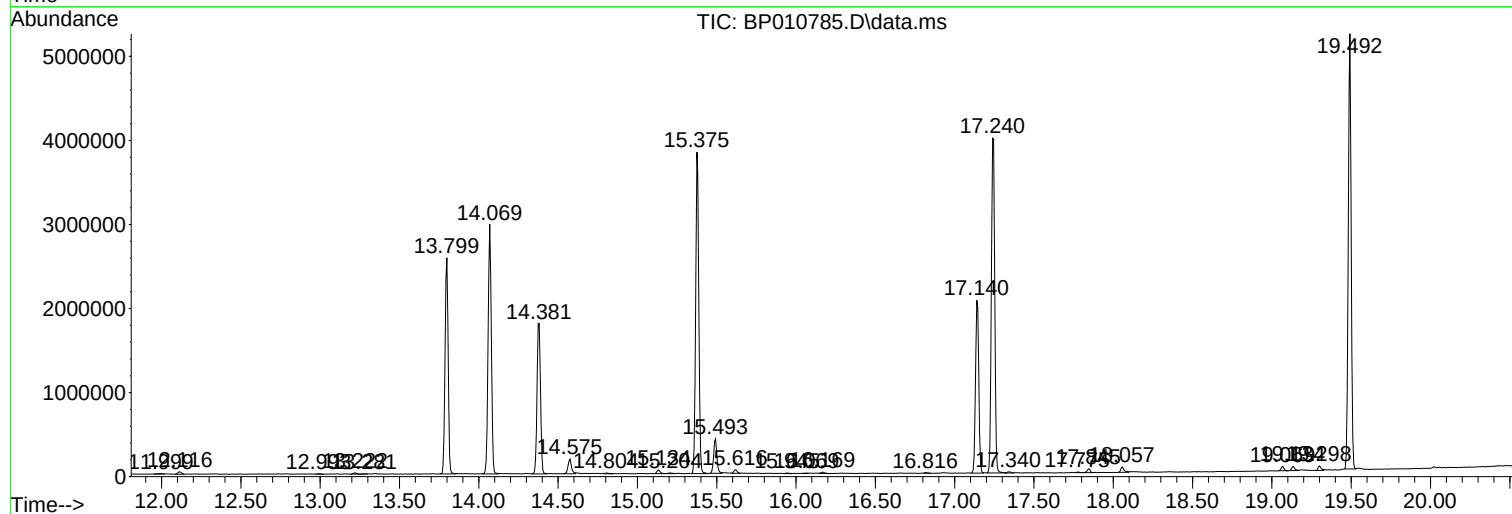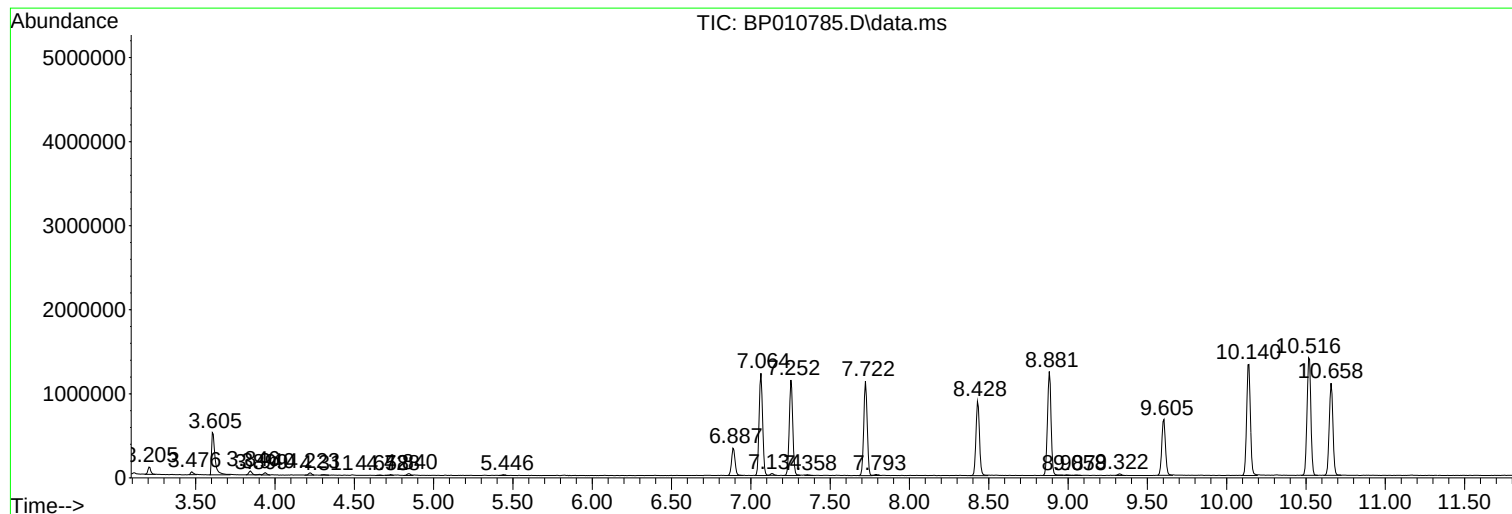

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010785.D
Acq On : 24 Jun 2022 10:30
Operator : CG/JU
Sample : N3395-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0158

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010785.D
Acq On : 24 Jun 2022 10:30
Operator : CG/JU
Sample : N3395-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0158

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------