

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010786.D
 Acq On : 24 Jun 2022 11:04
 Operator : CG/JU
 Sample : N3395-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0154

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	29	rVB	100849	132994	1.55%	0.152%
2	3.611	86	89	109	rBV	400203	556721	6.50%	0.637%
3	3.846	123	129	135	rBV	57233	85251	1.00%	0.098%
4	3.899	135	138	141	rVV4	10341	15421	0.18%	0.018%
5	3.940	141	145	151	rVB	47603	61199	0.71%	0.070%
6	4.311	204	208	214	rVB4	7319	10298	0.12%	0.012%
7	4.487	234	238	243	rVB3	10410	13925	0.16%	0.016%
8	4.728	275	279	283	rBV4	11546	14757	0.17%	0.017%
9	4.846	294	299	306	rBV	23759	40070	0.47%	0.046%
10	5.446	397	401	409	rVB	10686	18587	0.22%	0.021%
11	6.887	640	646	658	rBV	396679	605657	7.07%	0.693%
12	7.063	669	676	685	rVV	1640004	2409499	28.15%	2.758%
13	7.134	685	688	694	rVB2	7686	12679	0.15%	0.015%
14	7.252	700	708	722	rBV	1471143	2251266	26.30%	2.577%
15	7.352	722	725	730	rVB5	9344	13105	0.15%	0.015%
16	7.722	781	788	796	rVV	1563371	2400963	28.05%	2.749%
17	7.793	797	800	807	rVB5	6937	10853	0.13%	0.012%
18	8.428	901	908	920	rBV	1134888	1769228	20.67%	2.025%
19	8.881	978	985	996	rBV	1714086	2696543	31.50%	3.087%
20	9.322	1055	1060	1065	rVB4	8784	14307	0.17%	0.016%
21	9.605	1098	1108	1118	rBV	1014789	1605977	18.76%	1.838%
22	10.140	1190	1199	1210	rBV	1826057	2919703	34.11%	3.342%
23	10.522	1255	1264	1274	rVB	2078516	3481271	40.66%	3.985%
24	10.657	1277	1287	1299	rBV	1749964	2892009	33.78%	3.311%
25	12.116	1527	1535	1541	rBV	40558	68018	0.79%	0.078%
26	12.993	1680	1684	1688	rVB6	7860	11449	0.13%	0.013%
27	13.110	1698	1704	1707	rBV7	5817	11366	0.13%	0.013%
28	13.222	1719	1723	1728	rVB6	8545	12725	0.15%	0.015%
29	13.351	1738	1745	1748	rBV7	5034	9388	0.11%	0.011%
30	13.798	1814	1821	1831	rBV	3789734	5110797	59.70%	5.851%
31	14.069	1860	1867	1878	rBV	4189446	6105390	71.32%	6.989%
32	14.298	1903	1906	1910	rBV5	8490	9669	0.11%	0.011%
33	14.381	1910	1920	1927	rBV	2948413	4319102	50.45%	4.944%
34	14.575	1947	1953	1965	rBV	255183	390956	4.57%	0.448%
35	14.745	1978	1982	1987	rVB8	5117	9069	0.11%	0.010%
36	14.810	1987	1993	1999	rVB7	17065	28792	0.34%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010786.D
 Acq On : 24 Jun 2022 11:04
 Operator : CG/JU
 Sample : N3395-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0154

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	15.134	2043	2048	2053	rBV	42261	57838	0.68%	0.066%
38	15.204	2056	2060	2066	rVV3	9895	17332	0.20%	0.020%
39	15.257	2066	2069	2073	rVB2	13381	17080	0.20%	0.020%
40	15.381	2081	2090	2099	rBV	5166462	7616072	88.96%	8.719%
41	15.492	2103	2109	2122	rVV	896447	1268505	14.82%	1.452%
42	15.616	2126	2130	2137	rVB	59893	90908	1.06%	0.104%
43	15.951	2182	2187	2190	rBV7	7378	11142	0.13%	0.013%
44	16.128	2213	2217	2220	rBV4	19838	25682	0.30%	0.029%
45	16.169	2220	2224	2228	rVB6	22789	31252	0.37%	0.036%
46	16.663	2304	2308	2312	rBV5	7480	10095	0.12%	0.012%
47	16.816	2331	2334	2341	rVB7	10847	16194	0.19%	0.019%
48	16.928	2349	2353	2357	rBV2	22113	30576	0.36%	0.035%
49	17.139	2383	2389	2396	rBV	3225883	4628317	54.06%	5.298%
50	17.245	2400	2407	2422	rVB	5809689	8257312	96.45%	9.453%
51	17.675	2477	2480	2487	rVB4	11000	12557	0.15%	0.014%
52	17.834	2502	2507	2515	rBV4	17684	35349	0.41%	0.040%
53	18.057	2541	2545	2551	rBV2	65497	94512	1.10%	0.108%
54	18.128	2555	2557	2562	rVB2	10097	12758	0.15%	0.015%
55	19.069	2713	2717	2722	rVB2	66887	83484	0.98%	0.096%
56	19.133	2724	2728	2734	rBV	65659	89882	1.05%	0.103%
57	19.298	2753	2756	2762	rBV5	39158	55609	0.65%	0.064%
58	19.492	2783	2789	2795	rBV	6661257	8560896	100.00%	9.800%
59	20.986	3040	3043	3049	rBV4	87526	136532	1.59%	0.156%
60	21.251	3083	3088	3094	rBV	3493515	4147698	48.45%	4.748%
61	23.474	3458	3466	3481	rVB2	4101690	7761162	90.66%	8.885%
62	23.621	3484	3491	3501	rVB2	2050979	4166836	48.67%	4.770%




Sum of corrected areas: 87354584

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010786.D
Acq On : 24 Jun 2022 11:04
Operator : CG/JU
Sample : N3395-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

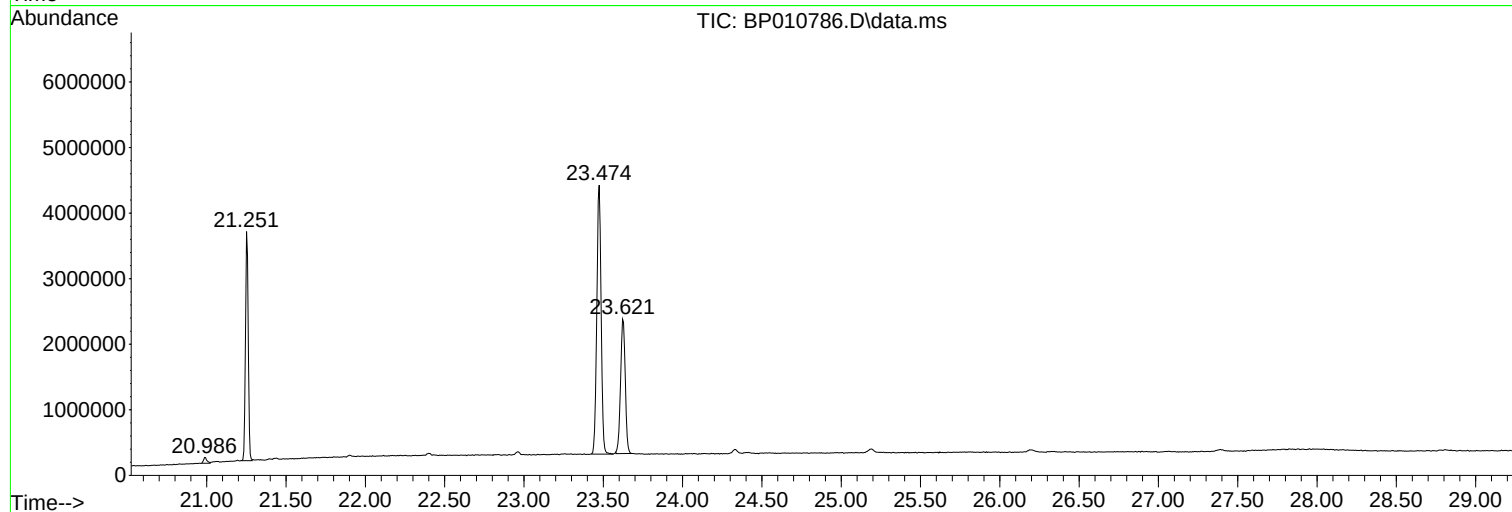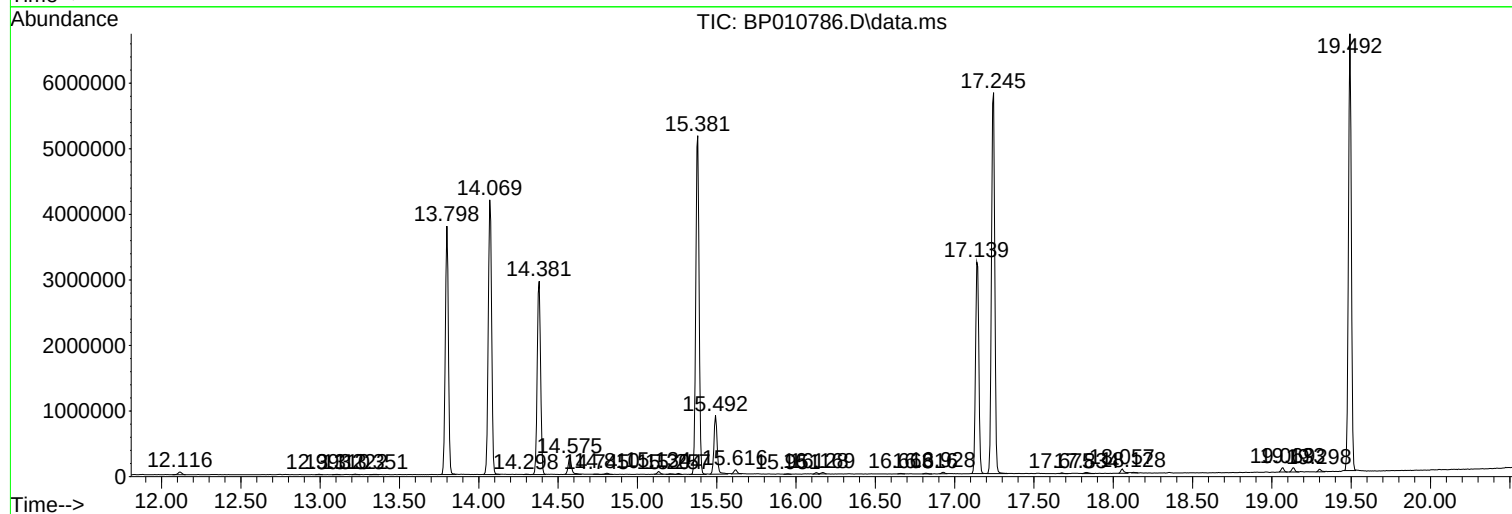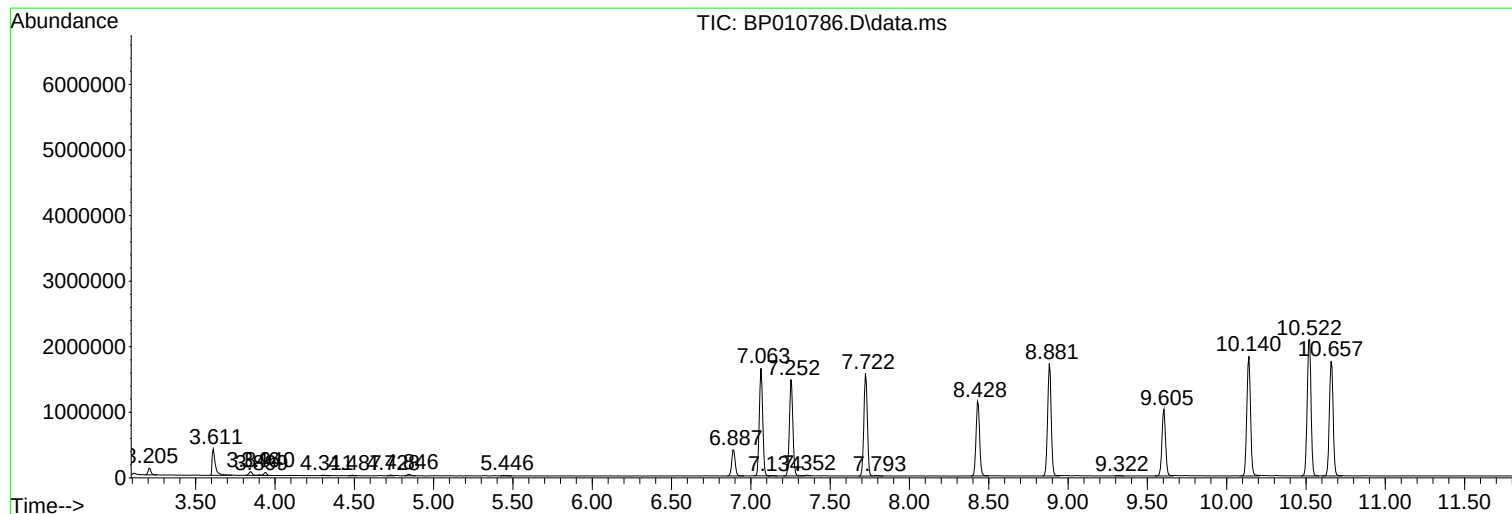

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010786.D
Acq On : 24 Jun 2022 11:04
Operator : CG/JU
Sample : N3395-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010786.D
Acq On : 24 Jun 2022 11:04
Operator : CG/JU
Sample : N3395-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
