

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010787.D
 Acq On : 24 Jun 2022 11:38
 Operator : CG/JU
 Sample : N3395-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	34	rVB	128169	180260	2.01%	0.203%
2	3.605	85	88	111	rBV	643109	953959	10.62%	1.076%
3	3.846	124	129	135	rBV	54691	81006	0.90%	0.091%
4	3.899	135	138	141	rVV4	8535	12303	0.14%	0.014%
5	3.940	141	145	151	rVB	31115	40844	0.45%	0.046%
6	4.487	235	238	246	rVB3	9229	16529	0.18%	0.019%
7	4.658	264	267	271	rBV3	8276	10898	0.12%	0.012%
8	4.728	275	279	283	rVV5	10442	15392	0.17%	0.017%
9	4.846	294	299	305	rBV	24764	42715	0.48%	0.048%
10	5.052	327	334	342	rBV	126340	189624	2.11%	0.214%
11	5.440	396	400	407	rVB2	11432	18474	0.21%	0.021%
12	6.887	640	646	655	rBV	676422	1030759	11.48%	1.163%
13	7.063	669	676	684	rBV	1805953	2690337	29.96%	3.035%
14	7.140	684	689	692	rVB	8754	14572	0.16%	0.016%
15	7.252	697	708	721	rBV	1748880	2690559	29.96%	3.035%
16	7.358	721	726	731	rVB6	9767	16503	0.18%	0.019%
17	7.610	761	769	777	rVV	54887	84867	0.94%	0.096%
18	7.722	781	788	805	rBV	1409845	2294931	25.55%	2.589%
19	8.069	843	847	853	rVB5	12209	21490	0.24%	0.024%
20	8.428	901	908	920	rBV	1466446	2291966	25.52%	2.585%
21	8.881	978	985	1000	rBV	1868462	2980585	33.19%	3.362%
22	9.322	1056	1060	1064	rVB3	9457	14250	0.16%	0.016%
23	9.604	1097	1108	1121	rBV	1134081	1837316	20.46%	2.073%
24	10.140	1190	1199	1208	rBV	2010315	3329468	37.07%	3.756%
25	10.381	1233	1240	1246	rVB	222003	352109	3.92%	0.397%
26	10.516	1255	1263	1272	rBV	1809665	2995799	33.36%	3.379%
27	10.657	1279	1287	1297	rBV	2070505	3345633	37.25%	3.774%
28	10.904	1323	1329	1339	rVB2	49350	89977	1.00%	0.101%
29	12.116	1529	1535	1541	rVB	45649	67970	0.76%	0.077%
30	13.216	1717	1722	1728	rBV7	9106	14837	0.17%	0.017%
31	13.798	1814	1821	1834	rBV	3777039	5099702	56.78%	5.753%
32	14.069	1858	1867	1875	rBV	4430795	6335743	70.55%	7.147%
33	14.375	1911	1919	1928	rVV	2360131	3477305	38.72%	3.922%
34	14.575	1946	1953	1964	rBV	391221	589133	6.56%	0.665%
35	14.740	1978	1981	1985	rVB6	7329	9539	0.11%	0.011%
36	14.804	1989	1992	1997	rVB6	13144	18977	0.21%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010787.D
 Acq On : 24 Jun 2022 11:38
 Operator : CG/JU
 Sample : N3395-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0157

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	15.134	2042	2048	2055	rBV	45789	63578	0.71%	0.072%
38	15.204	2056	2060	2066	rVB3	10767	18867	0.21%	0.021%
39	15.375	2083	2089	2103	rBV	5223619	7626126	84.92%	8.602%
40	15.492	2103	2109	2123	rBV	909112	1241358	13.82%	1.400%
41	15.616	2125	2130	2137	rVB	60288	95440	1.06%	0.108%
42	16.069	2202	2207	2214	rBV	5380	12992	0.14%	0.015%
43	16.169	2219	2224	2231	rBV4	22088	35024	0.39%	0.040%
44	16.822	2330	2335	2338	rVB5	9694	12727	0.14%	0.014%
45	17.139	2383	2389	2399	rBV	2564697	3548341	39.51%	4.003%
46	17.239	2399	2406	2417	rBV2	5527998	7894070	87.90%	8.905%
47	17.445	2439	2441	2446	rVB2	6587	9619	0.11%	0.011%
48	17.839	2502	2508	2512	rBV5	14407	29486	0.33%	0.033%
49	18.057	2541	2545	2548	rBV2	65943	89452	1.00%	0.101%
50	19.069	2712	2717	2721	rBV2	64813	85619	0.95%	0.097%
51	19.133	2724	2728	2734	rBV	60286	85264	0.95%	0.096%
52	19.298	2753	2756	2761	rBV3	44226	53531	0.60%	0.060%
53	19.492	2783	2789	2795	rBV	6314878	8198787	91.29%	9.248%
54	20.986	3040	3043	3047	rBV2	97016	125723	1.40%	0.142%
55	21.251	3083	3088	3094	rBV	2749786	3347830	37.28%	3.776%
56	23.474	3458	3466	3480	rVB2	4753613	8980798	100.00%	10.131%
57	23.627	3484	3492	3501	rVB2	1872106	3839762	42.76%	4.331%




Sum of corrected areas: 88650725

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010787.D
Acq On : 24 Jun 2022 11:38
Operator : CG/JU
Sample : N3395-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

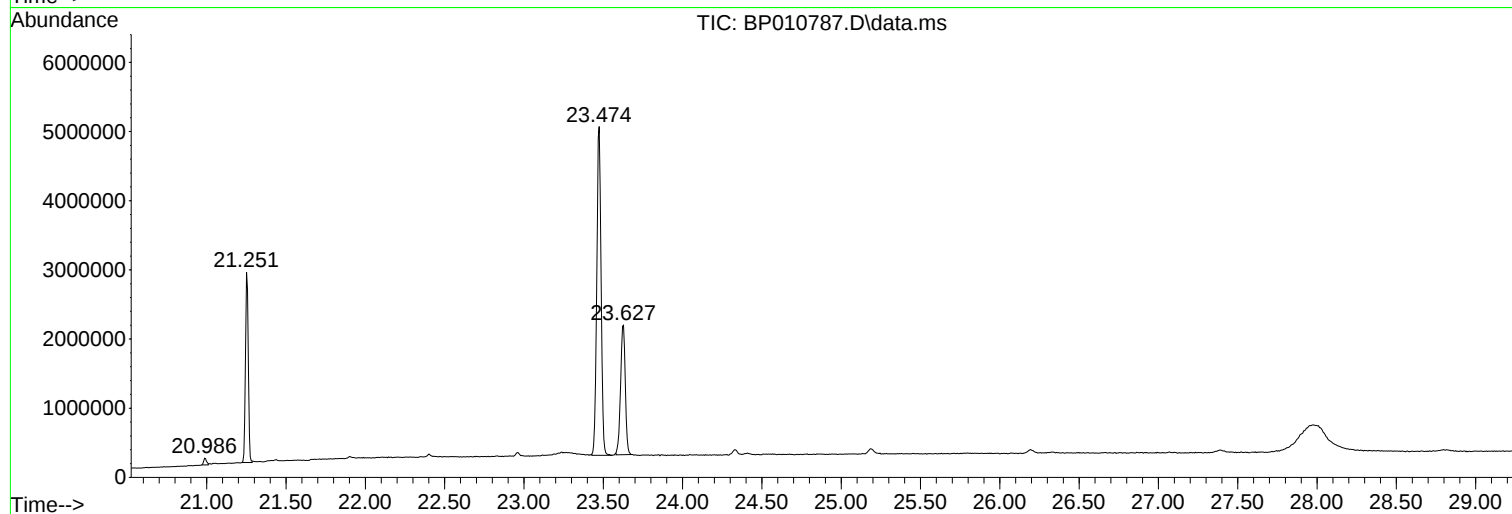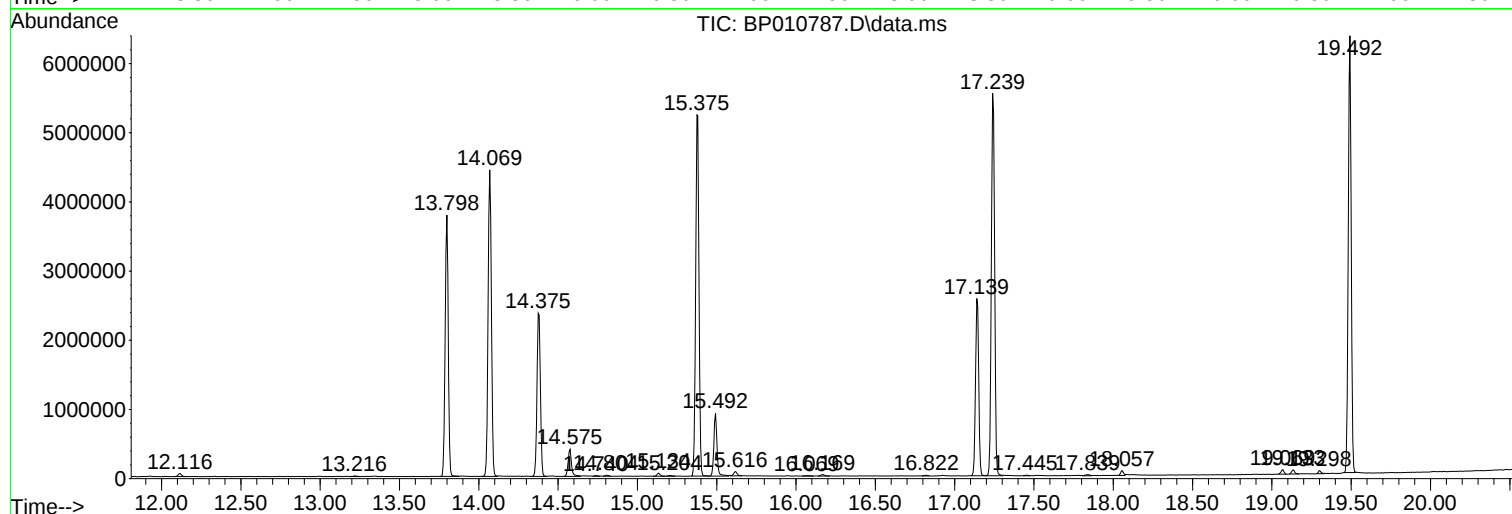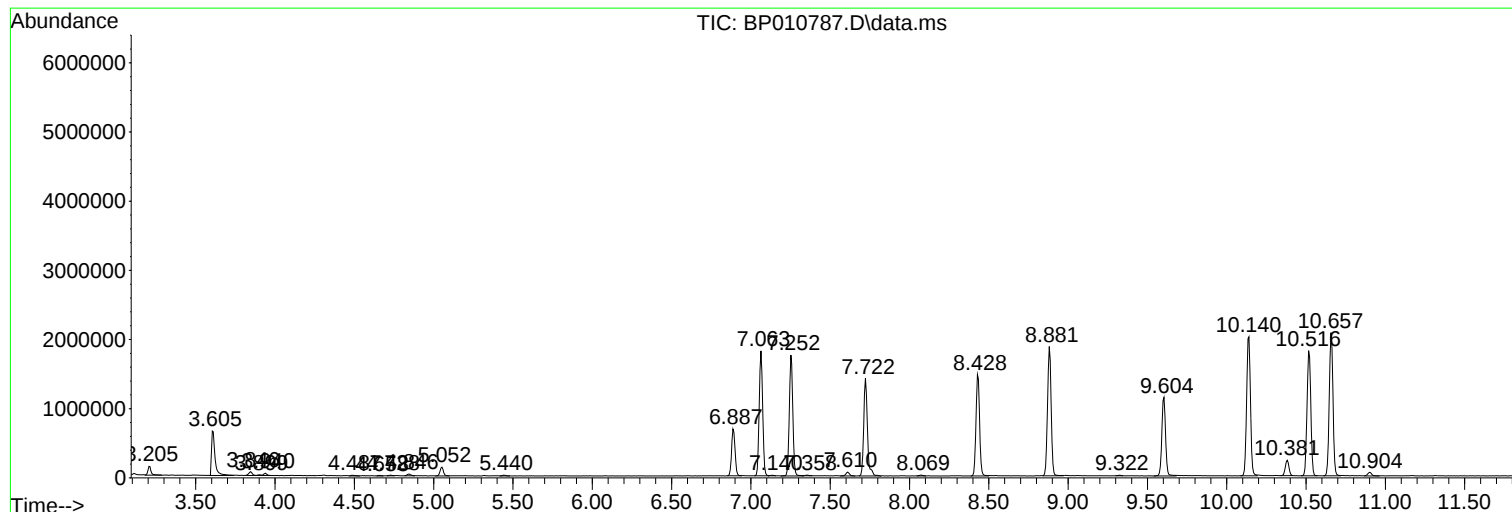

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010787.D
Acq On : 24 Jun 2022 11:38
Operator : CG/JU
Sample : N3395-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010787.D
Acq On : 24 Jun 2022 11:38
Operator : CG/JU
Sample : N3395-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0157

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc