

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010791.D
 Acq On : 24 Jun 2022 13:53
 Operator : CG/JU
 Sample : N3395-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0159

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	33	rVB	123434	162271	1.99%	0.195%
2	3.475	64	66	70	rBV3	8152	9630	0.12%	0.012%
3	3.605	86	88	105	rBV	690767	997625	12.21%	1.201%
4	3.846	123	129	135	rBV	61804	94064	1.15%	0.113%
5	3.899	135	138	141	rVV4	10910	14089	0.17%	0.017%
6	3.940	141	145	151	rVB	31847	42418	0.52%	0.051%
7	4.305	204	207	212	rVB4	8468	9979	0.12%	0.012%
8	4.487	235	238	242	rVB3	8679	11468	0.14%	0.014%
9	4.658	264	267	273	rVB	6292	9723	0.12%	0.012%
10	4.728	273	279	282	rBV3	11318	15577	0.19%	0.019%
11	4.840	293	298	305	rBV2	32242	53704	0.66%	0.065%
12	5.446	397	401	405	rVB	11982	17623	0.22%	0.021%
13	6.887	639	646	658	rBV	459769	704090	8.61%	0.847%
14	7.063	667	676	683	rBV	1691809	2553832	31.25%	3.074%
15	7.134	685	688	694	rVB	18152	26485	0.32%	0.032%
16	7.252	701	708	720	rBV	1623721	2475316	30.29%	2.979%
17	7.352	722	725	733	rVB5	11073	16959	0.21%	0.020%
18	7.722	779	788	795	rBV	1398042	2134590	26.12%	2.569%
19	7.793	795	800	810	rVB4	13776	22034	0.27%	0.027%
20	8.428	901	908	919	rBV	1255723	1940163	23.74%	2.335%
21	8.881	977	985	993	rBV	1815409	2835597	34.69%	3.413%
22	8.999	999	1005	1011	rVV3	31827	48939	0.60%	0.059%
23	9.322	1056	1060	1067	rBV	18429	28734	0.35%	0.035%
24	9.604	1099	1108	1118	rBV	1110009	1773682	21.70%	2.135%
25	10.134	1191	1198	1210	rBV	1896364	3078618	37.67%	3.706%
26	10.310	1227	1228	1234	rVB6	6557	8249	0.10%	0.010%
27	10.516	1253	1263	1271	rBV	1828652	3022558	36.98%	3.638%
28	10.657	1278	1287	1299	rBV	2015664	3319727	40.62%	3.996%
29	12.116	1528	1535	1542	rVB	43899	71399	0.87%	0.086%
30	12.328	1567	1571	1577	rVB7	5251	9587	0.12%	0.012%
31	13.216	1719	1722	1729	rVB4	16830	23159	0.28%	0.028%
32	13.345	1740	1744	1751	rVB7	6610	13313	0.16%	0.016%
33	13.704	1802	1805	1812	rVB9	6601	9989	0.12%	0.012%
34	13.798	1814	1821	1832	rBV	3503125	4668984	57.13%	5.620%
35	14.069	1858	1867	1877	rBV	4068274	5898603	72.17%	7.100%
36	14.375	1911	1919	1927	rBV	2369538	3534448	43.24%	4.254%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010791.D
 Acq On : 24 Jun 2022 13:53
 Operator : CG/JU
 Sample : N3395-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0159

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	14.575	1942	1953	1969	rBV	253751	412536	5.05%	0.497%
38	14.804	1989	1992	1997	rVB7	15687	22128	0.27%	0.027%
39	15.204	2055	2060	2067	rBV4	11753	23115	0.28%	0.028%
40	15.375	2082	2089	2100	rBV	4942395	7084399	86.68%	8.527%
41	15.492	2102	2109	2118	rBV	710316	995114	12.18%	1.198%
42	15.616	2125	2130	2136	rVB	60251	90819	1.11%	0.109%
43	16.169	2219	2224	2231	rVB4	18875	34879	0.43%	0.042%
44	16.816	2330	2334	2340	rBV7	9349	15130	0.19%	0.018%
45	16.928	2348	2353	2356	rBV6	8771	16335	0.20%	0.020%
46	17.092	2375	2381	2383	rBV7	5579	11832	0.14%	0.014%
47	17.139	2383	2389	2398	rVV	2553179	3655959	44.73%	4.401%
48	17.239	2400	2406	2418	rVV2	5087445	7301425	89.33%	8.788%
49	17.345	2420	2424	2429	rVB4	23187	33821	0.41%	0.041%
50	17.845	2502	2509	2514	rBV	43086	68106	0.83%	0.082%
51	18.057	2540	2545	2551	rBV4	48421	75675	0.93%	0.091%
52	18.351	2592	2595	2598	rBV5	6534	10188	0.12%	0.012%
53	19.069	2712	2717	2722	rBV	60763	82482	1.01%	0.099%
54	19.133	2724	2728	2734	rBV2	58240	78931	0.97%	0.095%
55	19.298	2753	2756	2765	rBV6	32141	41037	0.50%	0.049%
56	19.492	2783	2789	2796	rBV	5923619	7614488	93.16%	9.165%
57	20.986	3040	3043	3051	rBV6	58701	94297	1.15%	0.114%
58	21.251	3083	3088	3097	rBV	2783480	3516166	43.02%	4.232%
59	23.474	3458	3466	3478	rVB	4331050	8173191	100.00%	9.838%
60	23.627	3483	3492	3503	rVB2	1952501	3970509	48.58%	4.779%




Sum of corrected areas: 83079788

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010791.D
Acq On : 24 Jun 2022 13:53
Operator : CG/JU
Sample : N3395-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0159

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

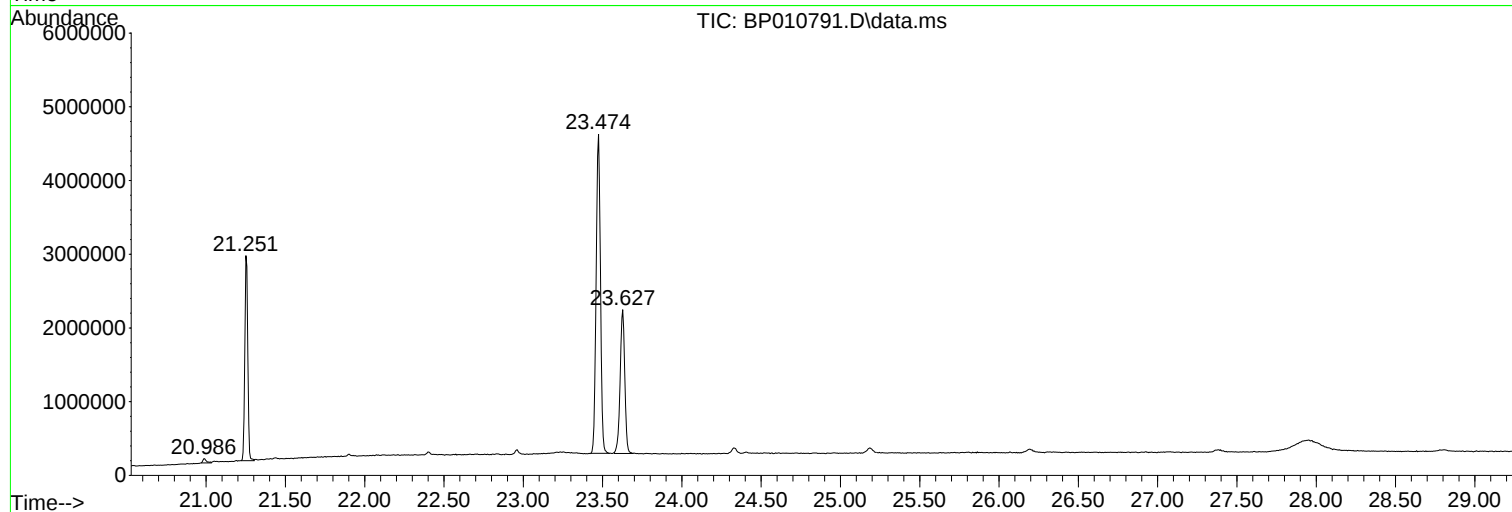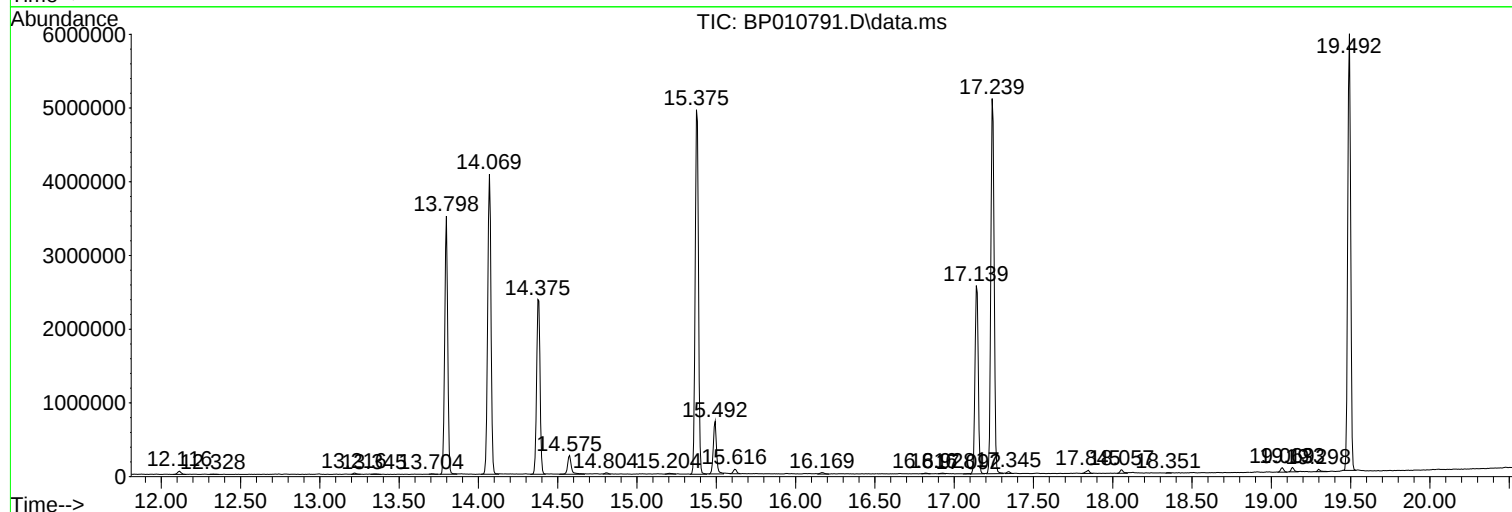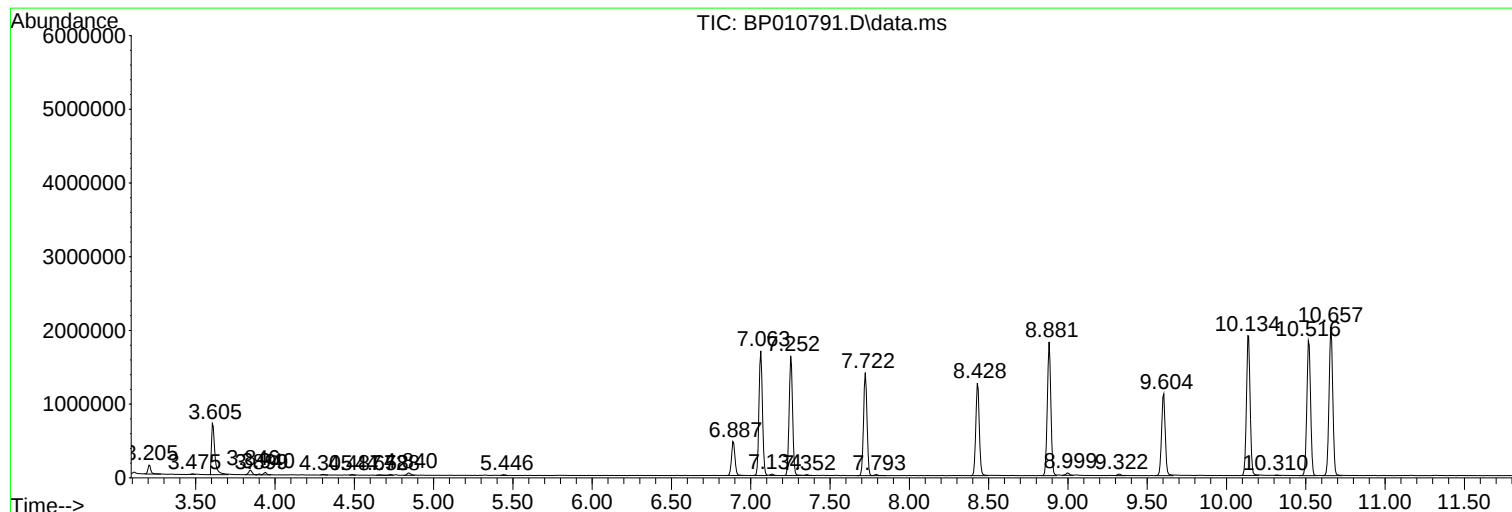

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010791.D
Acq On : 24 Jun 2022 13:53
Operator : CG/JU
Sample : N3395-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0159

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010791.D
Acq On : 24 Jun 2022 13:53
Operator : CG/JU
Sample : N3395-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0159

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------