

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010793.D
 Acq On : 24 Jun 2022 15:01
 Operator : CG/JU
 Sample : N3395-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0155

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010793.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	27	rBV	124394	160336	2.05%	0.182%
2	3.611	86	89	107	rBV	497505	732422	9.38%	0.830%
3	3.846	124	129	134	rBV	59616	90920	1.16%	0.103%
4	3.899	135	138	141	rVV4	10111	14298	0.18%	0.016%
5	3.940	141	145	152	rVB	52527	73191	0.94%	0.083%
6	4.299	204	206	213	rVB6	8964	12245	0.16%	0.014%
7	4.487	232	238	245	rVB4	8939	14109	0.18%	0.016%
8	4.658	263	267	272	rBV3	6362	9798	0.13%	0.011%
9	4.728	275	279	283	rBV5	11159	17423	0.22%	0.020%
10	4.764	283	285	289	rVB2	6292	8027	0.10%	0.009%
11	4.840	294	298	306	rBV	29804	46197	0.59%	0.052%
12	5.446	396	401	404	rBV	10664	14459	0.19%	0.016%
13	6.887	638	646	653	rBV	456951	698519	8.95%	0.791%
14	7.063	667	676	684	rBV	1748784	2626399	33.64%	2.976%
15	7.134	684	688	694	rVB	16311	25608	0.33%	0.029%
16	7.252	701	708	716	rBV	1669680	2518794	32.26%	2.854%
17	7.352	721	725	732	rVB3	10008	18539	0.24%	0.021%
18	7.722	779	788	795	rBV	1704450	2578521	33.03%	2.922%
19	7.799	795	801	804	rVV5	7432	10788	0.14%	0.012%
20	8.428	901	908	917	rBV	1271989	1964304	25.16%	2.226%
21	8.881	976	985	994	rBV	1890235	2957218	37.88%	3.351%
22	9.052	1010	1014	1020	rVB8	7395	10892	0.14%	0.012%
23	9.322	1057	1060	1070	rVB3	13752	20769	0.27%	0.024%
24	9.605	1099	1108	1119	rBV	1140313	1877437	24.05%	2.127%
25	10.134	1188	1198	1210	rBV	1948714	3195186	40.92%	3.620%
26	10.316	1222	1229	1233	rBV10	5357	8382	0.11%	0.009%
27	10.516	1254	1263	1273	rVB	2247634	3672493	47.04%	4.161%
28	10.657	1280	1287	1297	rBV	2015727	3223173	41.28%	3.652%
29	12.116	1528	1535	1544	rVB2	44473	77888	1.00%	0.088%
30	12.334	1568	1572	1578	rVB9	5824	10668	0.14%	0.012%
31	12.993	1679	1684	1690	rVB7	8327	13179	0.17%	0.015%
32	13.216	1716	1722	1727	rBV7	9451	16086	0.21%	0.018%
33	13.346	1739	1744	1749	rVB7	6582	11270	0.14%	0.013%
34	13.798	1814	1821	1835	rBV	3817431	5039864	64.55%	5.710%
35	14.069	1859	1867	1876	rBV	4352756	6229026	79.78%	7.058%
36	14.293	1901	1905	1910	rVB7	4793	9611	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010793.D
 Acq On : 24 Jun 2022 15:01
 Operator : CG/JU
 Sample : N3395-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0155

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	14.375	1912	1919	1927	rBV	2920913	4379235	56.09%	4.962%
38	14.575	1947	1953	1962	rBV	269660	410883	5.26%	0.466%
39	14.740	1977	1981	1985	rVB7	7000	11954	0.15%	0.014%
40	14.810	1987	1993	1998	rVB5	20337	32235	0.41%	0.037%
41	15.134	2043	2048	2055	rBV	20751	30108	0.39%	0.034%
42	15.204	2055	2060	2064	rBV2	13831	20193	0.26%	0.023%
43	15.375	2082	2089	2099	rBV	5246289	7582596	97.12%	8.591%
44	15.492	2102	2109	2119	rBV	924720	1255729	16.08%	1.423%
45	15.616	2126	2130	2136	rVB	59974	85765	1.10%	0.097%
46	16.169	2219	2224	2229	rVB4	20127	32541	0.42%	0.037%
47	16.816	2329	2334	2340	rBV6	10725	17134	0.22%	0.019%
48	16.922	2345	2352	2355	rBV4	11045	18738	0.24%	0.021%
49	17.139	2383	2389	2396	rBV	3224299	4530449	58.03%	5.133%
50	17.239	2400	2406	2417	rVV2	5660462	7807565	100.00%	8.846%
51	17.345	2420	2424	2428	rVB7	7413	10501	0.13%	0.012%
52	17.828	2503	2506	2514	rVB9	14788	29533	0.38%	0.033%
53	18.051	2540	2544	2549	rBV	66469	96953	1.24%	0.110%
54	18.351	2591	2595	2598	rBV6	6842	12461	0.16%	0.014%
55	19.069	2712	2717	2721	rBV2	60154	84121	1.08%	0.095%
56	19.133	2724	2728	2733	rVV	63616	79487	1.02%	0.090%
57	19.298	2752	2756	2761	rBV3	54424	70376	0.90%	0.080%
58	19.451	2779	2782	2783	rBV3	14098	13365	0.17%	0.015%
59	19.492	2783	2789	2795	rVV	6072539	7781368	99.66%	8.816%
60	21.251	3083	3088	3097	rBV	3150725	3926289	50.29%	4.449%
61	23.474	3458	3466	3477	rVB2	4004022	7637866	97.83%	8.654%
62	23.621	3483	3491	3502	rVB2	2068476	4294080	55.00%	4.865%




Sum of corrected areas: 88259564

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010793.D
Acq On : 24 Jun 2022 15:01
Operator : CG/JU
Sample : N3395-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0155

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

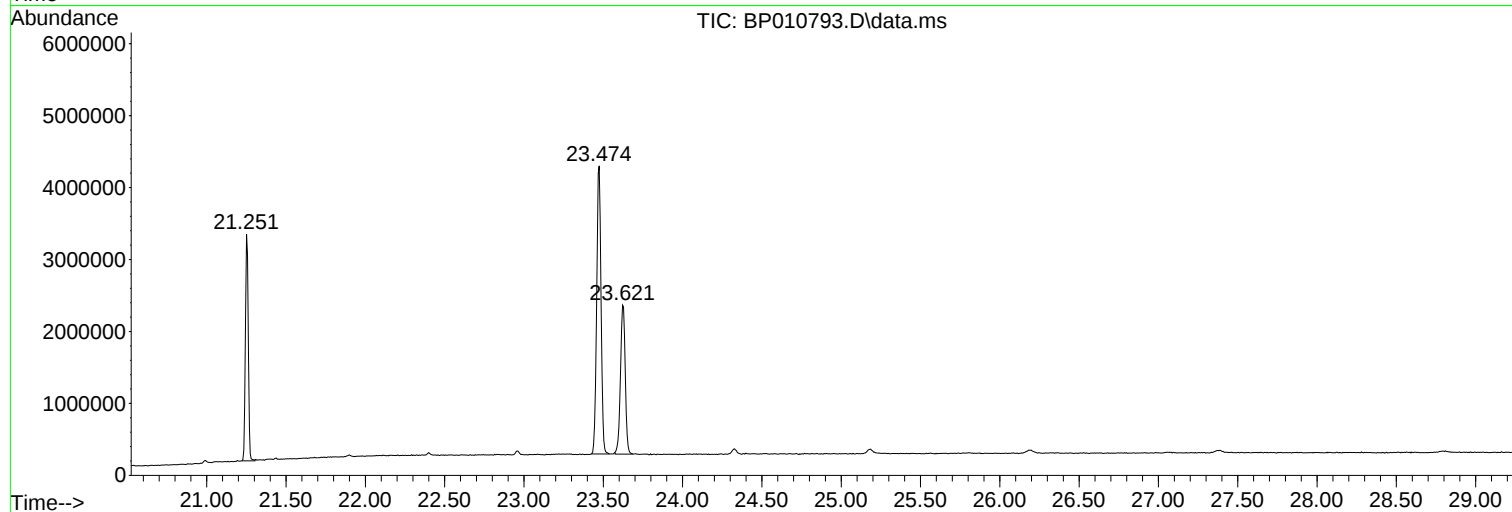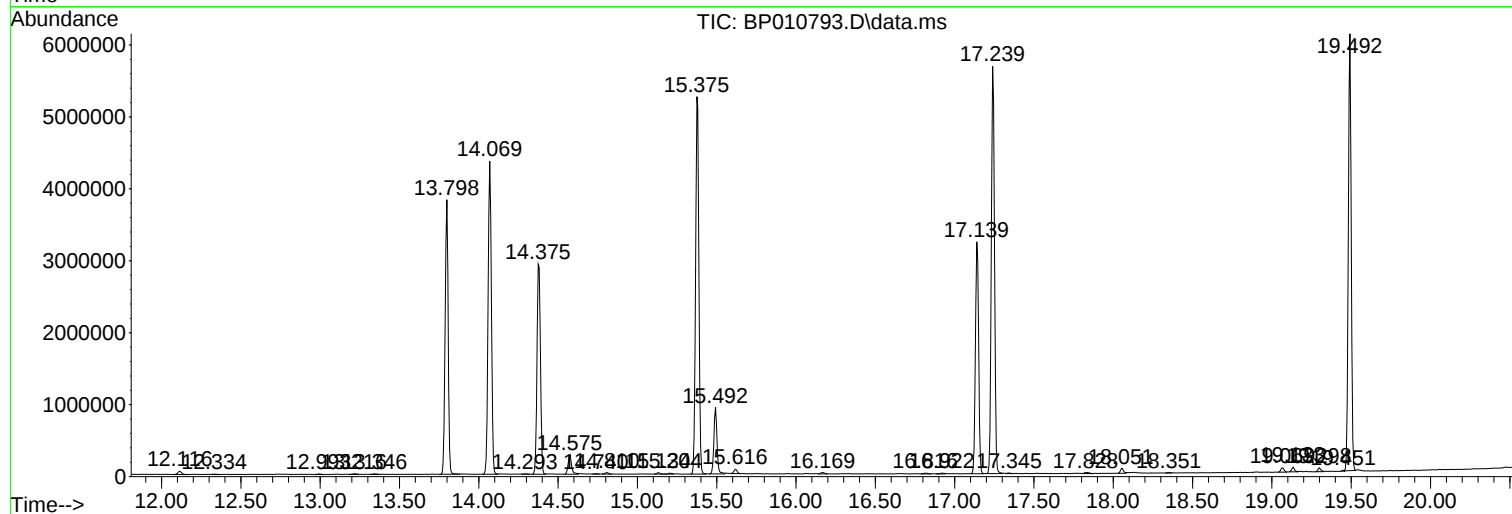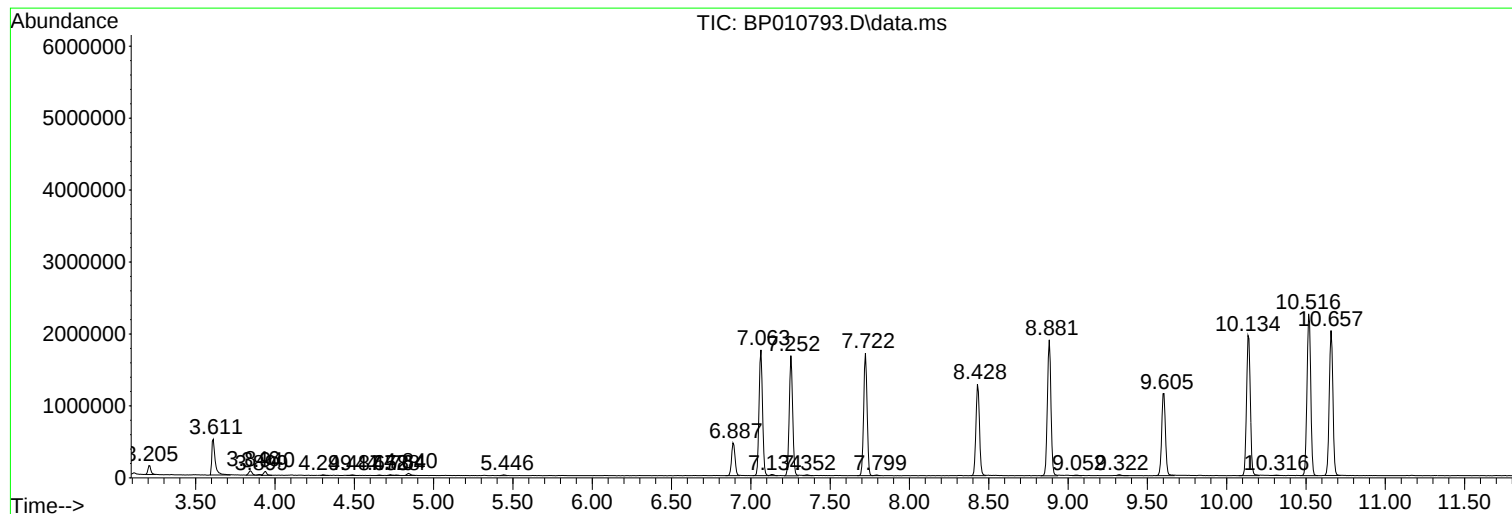

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010793.D
Acq On : 24 Jun 2022 15:01
Operator : CG/JU
Sample : N3395-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0155

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010793.D
Acq On : 24 Jun 2022 15:01
Operator : CG/JU
Sample : N3395-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0155

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc