

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010801.D
 Acq On : 24 Jun 2022 19:32
 Operator : CG/JU
 Sample : PB145724BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK724

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	29	rVB	155943	197422	2.06%	0.189%
2	3.605	85	88	112	rBV	1952836	2710991	28.29%	2.602%
3	3.934	140	144	150	rVB	30764	41103	0.43%	0.039%
4	4.158	179	182	187	rVB4	9307	11682	0.12%	0.011%
5	6.887	639	646	660	rBV	2030671	3121238	32.57%	2.996%
6	7.064	669	676	687	rVB	1751933	2631115	27.45%	2.525%
7	7.252	700	708	724	rBV	2090619	3200156	33.39%	3.071%
8	7.722	779	788	796	rBV	1565398	2400080	25.04%	2.303%
9	8.428	901	908	919	rBV	2483363	3915895	40.86%	3.758%
10	8.881	977	985	994	rBV	1911955	2993663	31.24%	2.873%
11	9.599	1097	1107	1121	rBV	1239469	2016581	21.04%	1.935%
12	10.134	1189	1198	1217	rBV	2265006	3640164	37.98%	3.494%
13	10.516	1254	1263	1271	rBV	2166958	3530921	36.84%	3.389%
14	10.657	1279	1287	1298	rBV	2538837	4172386	43.54%	4.004%
15	12.110	1528	1534	1539	rBV	47355	78146	0.82%	0.075%
16	13.346	1737	1744	1751	rVB6	6782	14049	0.15%	0.013%
17	13.798	1814	1821	1835	rBV	4340003	5702716	59.51%	5.473%
18	14.069	1856	1867	1881	rBV	4898335	6854728	71.53%	6.579%
19	14.375	1912	1919	1926	rBV	3071576	4482363	46.77%	4.302%
20	14.575	1946	1953	1966	rBV	1814959	2553979	26.65%	2.451%
21	14.804	1988	1992	1998	rVB8	7794	13534	0.14%	0.013%
22	15.198	2057	2059	2065	rVB7	5745	10042	0.10%	0.010%
23	15.375	2082	2089	2099	rBV	5880931	8402995	87.68%	8.065%
24	15.493	2102	2109	2125	rVV	1147783	1587455	16.56%	1.524%
25	15.616	2125	2130	2143	rVB	73677	124110	1.30%	0.119%
26	16.163	2219	2223	2231	rVB5	22159	34085	0.36%	0.033%
27	16.816	2326	2334	2339	rBV10	12112	26089	0.27%	0.025%
28	16.922	2347	2352	2356	rBV6	8758	12731	0.13%	0.012%
29	17.139	2383	2389	2399	rBV	3747922	5018918	52.37%	4.817%
30	17.239	2399	2406	2420	rBV2	6328233	8777015	91.58%	8.423%
31	17.828	2503	2506	2512	rVB8	7200	11111	0.12%	0.011%
32	18.051	2540	2544	2548	rBV6	14890	21057	0.22%	0.020%
33	18.904	2687	2689	2696	rVB8	11452	16760	0.17%	0.016%
34	19.063	2712	2716	2722	rBV2	76847	101806	1.06%	0.098%
35	19.134	2723	2728	2733	rVV	68037	94855	0.99%	0.091%
36	19.298	2753	2756	2759	rBV4	11433	15367	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010801.D
Acq On : 24 Jun 2022 19:32
Operator : CG/JU
Sample : PB145724BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK724

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

37	19.492	2783	2789	2796	rBV	7163805	9583547	100.00%	9.198%
38	21.251	3083	3088	3096	rBV	3868396	4572848	47.72%	4.389%
39	23.469	3457	3465	3475	rBV2	3901223	7483270	78.08%	7.182%
40	23.622	3484	3491	3502	rVB	2098439	4020027	41.95%	3.858%




Sum of corrected areas: 104197000

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010801.D
Acq On : 24 Jun 2022 19:32
Operator : CG/JU
Sample : PB145724BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

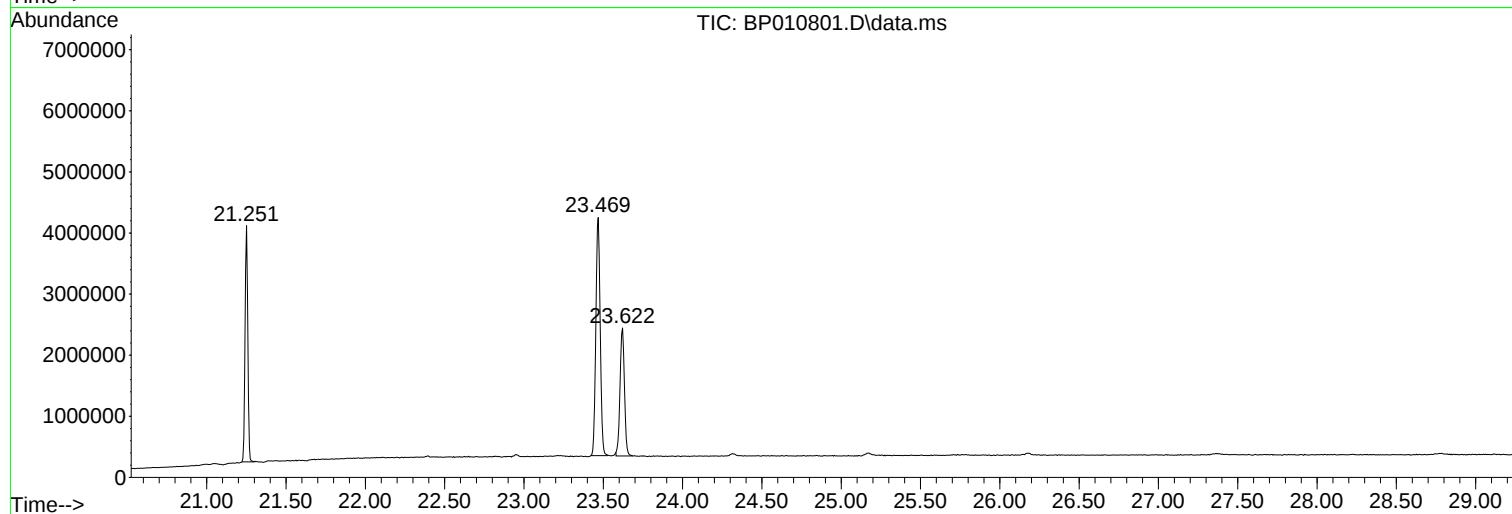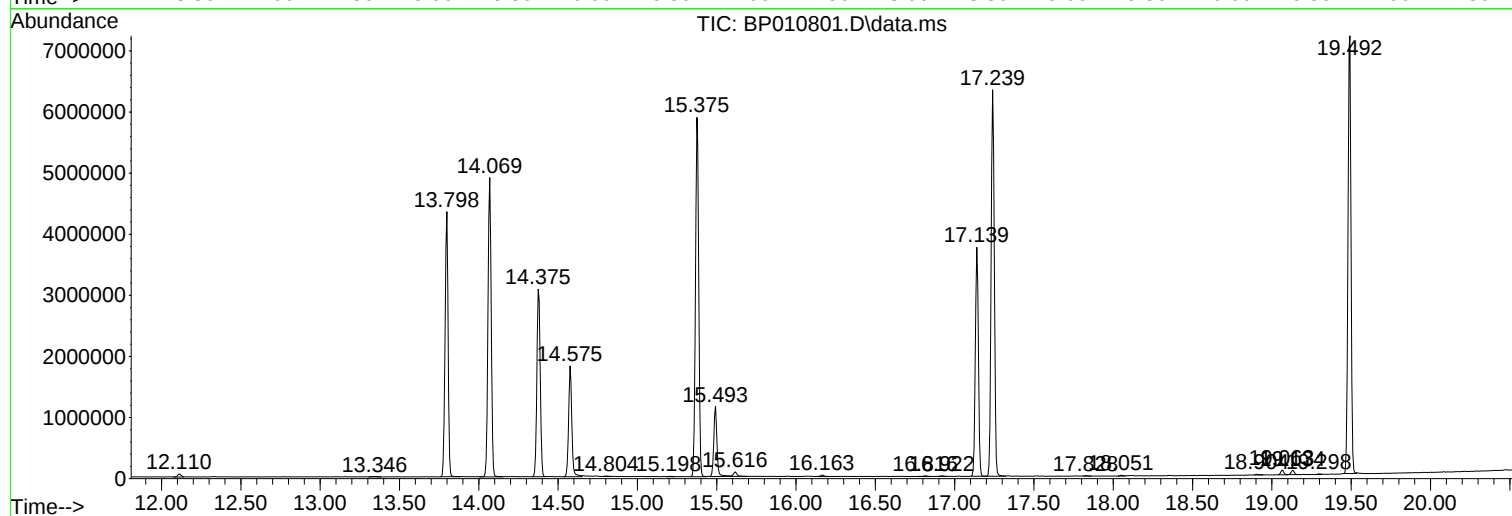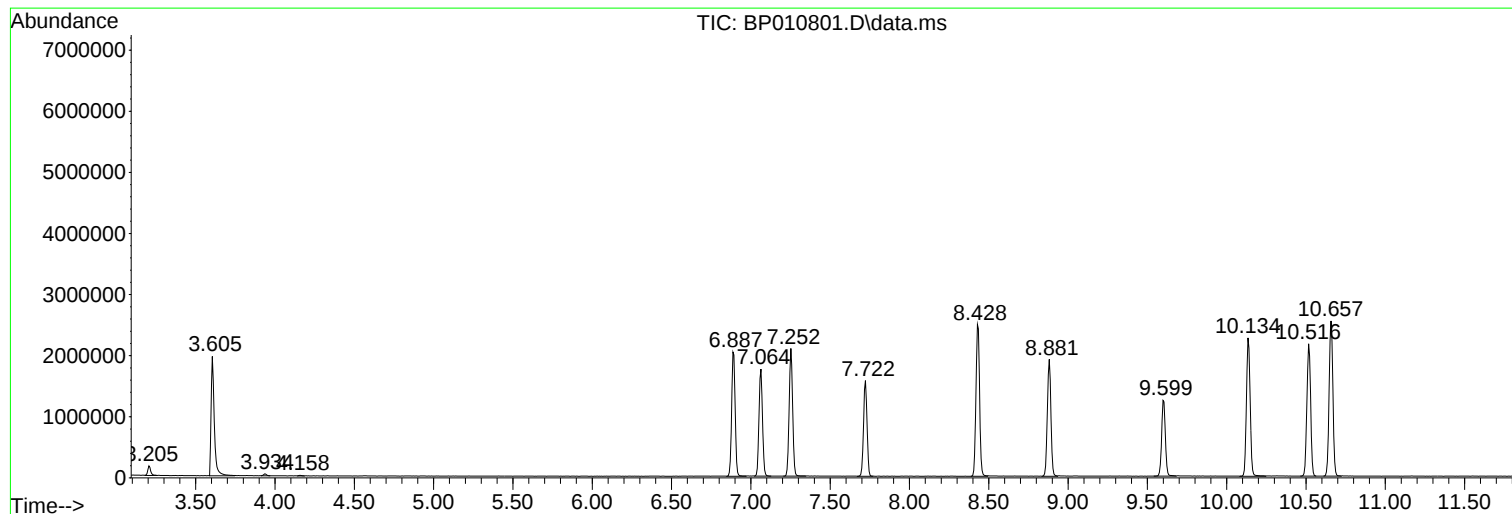

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010801.D
Acq On : 24 Jun 2022 19:32
Operator : CG/JU
Sample : PB145724BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010801.D
Acq On : 24 Jun 2022 19:32
Operator : CG/JU
Sample : PB145724BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------