

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010802.D
 Acq On : 24 Jun 2022 20:06
 Operator : CG/JU
 Sample : PB145730BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK730

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010802.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	29	rVB	163669	201964	2.71%	0.213%
2	3.605	84	88	112	rBV	2017963	2746950	36.81%	2.893%
3	3.940	141	145	154	rVB	36048	56025	0.75%	0.059%
4	4.158	178	182	187	rBV4	9052	13458	0.18%	0.014%
5	6.887	639	646	658	rBV	1999584	3081046	41.29%	3.245%
6	7.063	669	676	685	rVB	1730838	2607528	34.95%	2.746%
7	7.252	699	708	717	rBV	2112112	3185716	42.69%	3.355%
8	7.722	779	788	800	rVB	1645322	2509947	33.64%	2.644%
9	8.428	900	908	923	rBV	2423259	3833130	51.37%	4.037%
10	8.881	977	985	993	rBV	1900561	2923461	39.18%	3.079%
11	9.598	1099	1107	1121	rBV	1189689	1916560	25.69%	2.019%
12	10.134	1190	1198	1217	rBV	2122081	3510871	47.05%	3.698%
13	10.516	1255	1263	1271	rBV	2182412	3611941	48.41%	3.804%
14	10.657	1279	1287	1295	rBV	2438815	3957935	53.04%	4.169%
15	12.110	1526	1534	1541	rBV	42099	71864	0.96%	0.076%
16	12.328	1567	1571	1575	rVB7	5830	8045	0.11%	0.008%
17	13.345	1738	1744	1747	rBV6	5186	8709	0.12%	0.009%
18	13.798	1814	1821	1832	rBV	3672350	4924153	65.99%	5.187%
19	14.069	1858	1867	1875	rBV	4279830	6221438	83.38%	6.553%
20	14.375	1912	1919	1928	rBV	3078200	4385214	58.77%	4.619%
21	14.575	1946	1953	1970	rBV	1505599	2124156	28.47%	2.237%
22	14.739	1979	1981	1986	rVB6	6117	7477	0.10%	0.008%
23	14.804	1989	1992	1995	rVB5	5797	7527	0.10%	0.008%
24	15.204	2054	2060	2066	rBV10	5425	12210	0.16%	0.013%
25	15.375	2081	2089	2098	rBV	5225806	7354520	98.56%	7.746%
26	15.492	2103	2109	2121	rVV	902044	1226122	16.43%	1.291%
27	15.616	2125	2130	2139	rVB2	62045	97992	1.31%	0.103%
28	15.945	2181	2186	2190	rBV7	5670	10091	0.14%	0.011%
29	16.169	2219	2224	2230	rVB2	20996	30547	0.41%	0.032%
30	16.816	2330	2334	2339	rBV7	11595	15070	0.20%	0.016%
31	16.922	2348	2352	2356	rBV5	8641	11905	0.16%	0.013%
32	17.139	2382	2389	2398	rBV	3326206	4583480	61.43%	4.828%
33	17.239	2399	2406	2416	rBV2	5330420	7281621	97.59%	7.670%
34	18.051	2541	2544	2548	rBV5	11517	16430	0.22%	0.017%
35	18.357	2592	2596	2599	rBV6	5640	9950	0.13%	0.010%
36	18.904	2687	2689	2693	rBV4	7230	7690	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010802.D
Acq On : 24 Jun 2022 20:06
Operator : CG/JU
Sample : PB145730BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK730

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

37	19.063	2712	2716	2722	rBV	58084	78951	1.06%	0.083%
38	19.133	2723	2728	2733	rBV	55595	76759	1.03%	0.081%
39	19.298	2753	2756	2759	rBV5	8104	10468	0.14%	0.011%
40	19.492	2783	2789	2795	rBV	5717018	7461594	100.00%	7.859%
41	21.251	3083	3088	3098	rBV	3295342	3937050	52.76%	4.147%
42	23.468	3458	3465	3478	rVB2	3580467	6757112	90.56%	7.117%
43	23.621	3484	3491	3503	rVB2	2027866	4046063	54.23%	4.262%




Sum of corrected areas: 94940740

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010802.D
Acq On : 24 Jun 2022 20:06
Operator : CG/JU
Sample : PB145730BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK730

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

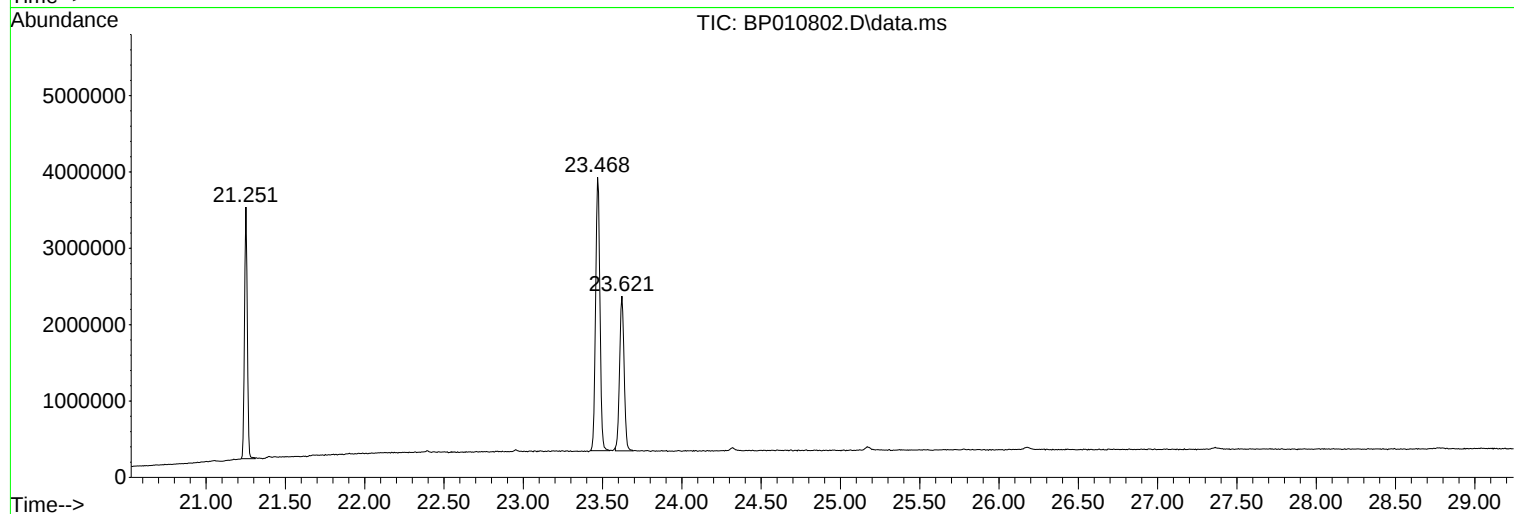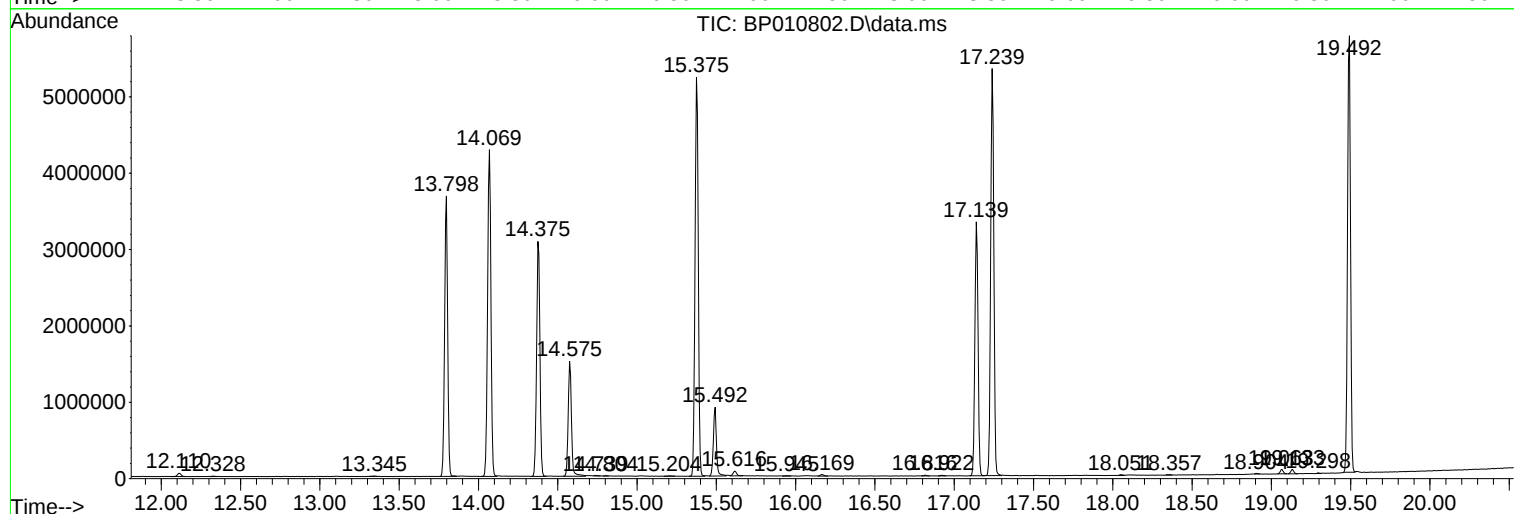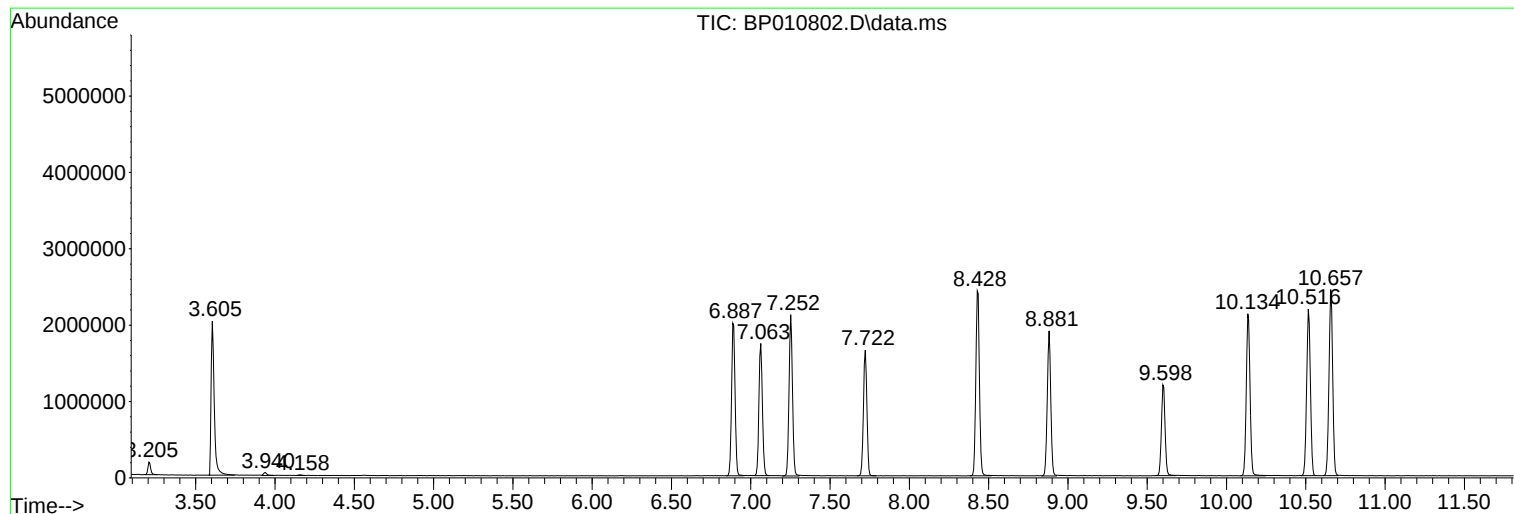

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010802.D
Acq On : 24 Jun 2022 20:06
Operator : CG/JU
Sample : PB145730BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK730

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010802.D
Acq On : 24 Jun 2022 20:06
Operator : CG/JU
Sample : PB145730BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK730

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------