

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010807.D
 Acq On : 24 Jun 2022 22:55
 Operator : CG/JU
 Sample : N3401-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	36	rVB	115327	162615	1.59%	0.179%
2	3.610	86	89	106	rBV	574437	826952	8.09%	0.910%
3	3.846	124	129	133	rBV	51640	77404	0.76%	0.085%
4	3.934	141	144	152	rVB	30346	44296	0.43%	0.049%
5	4.487	235	238	243	rVB4	8274	12670	0.12%	0.014%
6	4.728	275	279	282	rVB3	9849	12376	0.12%	0.014%
7	4.840	291	298	305	rBV2	26088	51021	0.50%	0.056%
8	5.434	396	399	406	rVB2	11367	18459	0.18%	0.020%
9	6.887	640	646	658	rVB	415186	649199	6.35%	0.715%
10	7.063	669	676	684	rBV	1603292	2460428	24.08%	2.709%
11	7.134	684	688	695	rVB	21129	33190	0.32%	0.037%
12	7.251	700	708	716	rBV	1537719	2352527	23.02%	2.590%
13	7.351	723	725	733	rVB7	8943	12704	0.12%	0.014%
14	7.722	780	788	795	rBV	1309393	1996313	19.54%	2.198%
15	7.787	795	799	806	rVB	21192	32110	0.31%	0.035%
16	8.428	901	908	920	rBV	1204919	1878432	18.38%	2.068%
17	8.881	975	985	995	rBV	1784226	2833507	27.73%	3.120%
18	8.992	999	1004	1008	rVV2	19302	34649	0.34%	0.038%
19	9.316	1053	1059	1066	rVB2	40119	62643	0.61%	0.069%
20	9.598	1099	1107	1117	rBV	1174505	1867065	18.27%	2.056%
21	10.134	1190	1198	1216	rBV	1935795	3123786	30.57%	3.439%
22	10.516	1254	1263	1272	rBV	1719760	2835328	27.75%	3.122%
23	10.657	1279	1287	1298	rBV	1962013	3152110	30.85%	3.470%
24	11.969	1505	1510	1512	rBV2	9736	13387	0.13%	0.015%
25	12.110	1529	1534	1541	rVB	42713	69768	0.68%	0.077%
26	12.781	1644	1648	1653	rVB8	7952	12104	0.12%	0.013%
27	13.216	1716	1722	1727	rBV3	28415	38435	0.38%	0.042%
28	13.798	1813	1821	1829	rBV	3675005	5032140	49.25%	5.540%
29	14.069	1857	1867	1878	rBV	4332449	6213758	60.81%	6.841%
30	14.298	1899	1906	1909	rBV7	8471	12450	0.12%	0.014%
31	14.375	1911	1919	1926	rBV	2396088	3458279	33.84%	3.807%
32	14.575	1946	1953	1967	rBV	317103	476674	4.67%	0.525%
33	14.739	1977	1981	1988	rVB10	8271	12197	0.12%	0.013%
34	14.804	1988	1992	2001	rVB10	14394	23410	0.23%	0.026%
35	15.133	2042	2048	2053	rBV	53552	76082	0.74%	0.084%
36	15.375	2082	2089	2100	rBV	5352837	7649667	74.86%	8.422%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
 Data File : BP010807.D
 Acq On : 24 Jun 2022 22:55
 Operator : CG/JU
 Sample : N3401-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	15.492	2103	2109	2124	rVV	992287	1418551	13.88%	1.562%
38	15.616	2126	2130	2142	rVB3	71157	111038	1.09%	0.122%
39	15.945	2182	2186	2191	rVB8	6200	10603	0.10%	0.012%
40	16.169	2219	2224	2230	rVB4	21227	31846	0.31%	0.035%
41	16.816	2329	2334	2339	rVB8	10321	17491	0.17%	0.019%
42	16.921	2348	2352	2356	rBV7	11757	21619	0.21%	0.024%
43	17.139	2382	2389	2399	rBV	2816850	3928132	38.44%	4.325%
44	17.239	2399	2406	2419	rBV	5896064	8107930	79.35%	8.926%
45	17.833	2502	2507	2512	rVB8	12931	21768	0.21%	0.024%
46	18.051	2539	2544	2549	rBV2	107706	144439	1.41%	0.159%
47	18.251	2574	2578	2590	rBV2	51188	82180	0.80%	0.090%
48	18.345	2590	2594	2600	rVV9	11852	21904	0.21%	0.024%
49	19.063	2712	2716	2722	rBV	76214	102874	1.01%	0.113%
50	19.133	2723	2728	2733	rVV	70600	103499	1.01%	0.114%
51	19.192	2736	2738	2746	rVB9	12600	23717	0.23%	0.026%
52	19.298	2752	2756	2760	rBV	61711	82415	0.81%	0.091%
53	19.439	2776	2780	2783	rBV4	34497	53086	0.52%	0.058%
54	19.486	2783	2788	2795	rVV	7426591	9364873	91.65%	10.310%
55	20.980	3039	3042	3050	rBV2	146401	233219	2.28%	0.257%
56	21.251	3083	3088	3093	rBV	3709864	4419533	43.25%	4.866%
57	23.468	3457	3465	3477	rVB	5496615	10218035	100.00%	11.249%
58	23.621	3484	3491	3500	rVB2	2320061	4694295	45.94%	5.168%




Sum of corrected areas: 90831182

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010807.D
Acq On : 24 Jun 2022 22:55
Operator : CG/JU
Sample : N3401-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

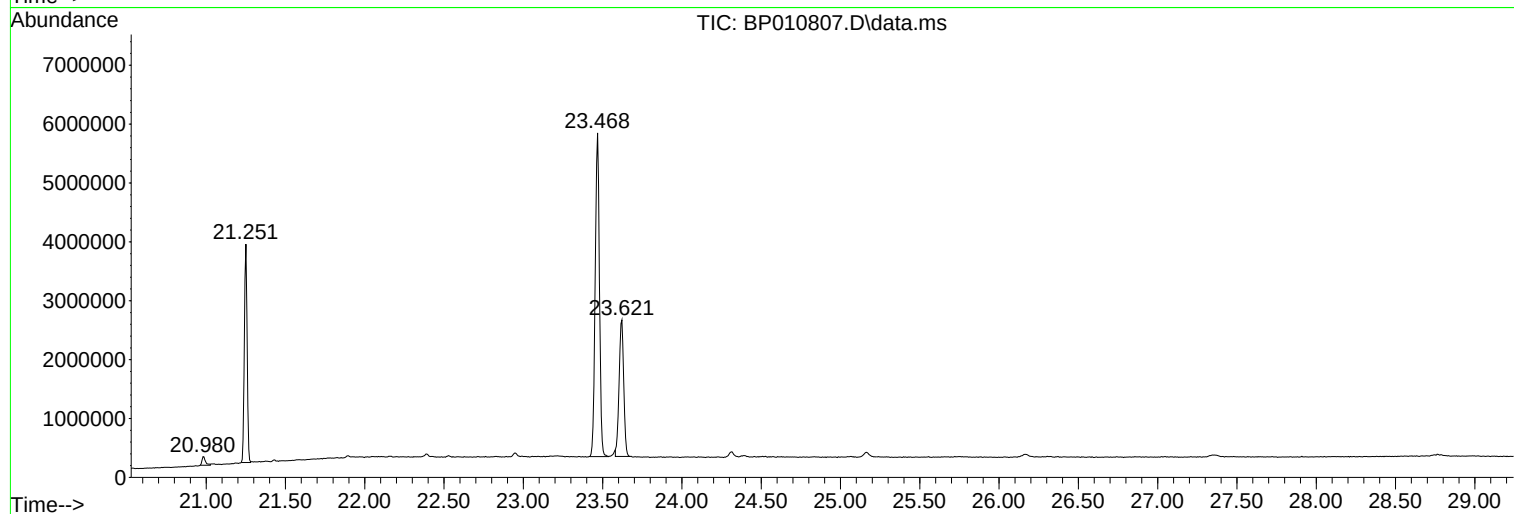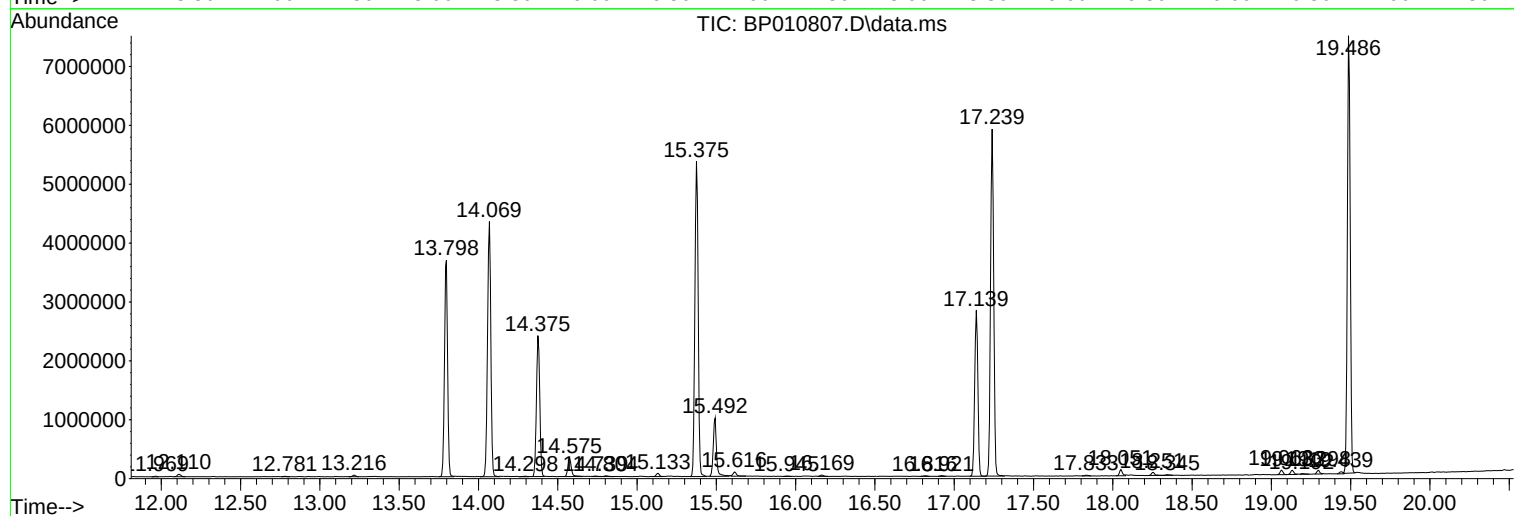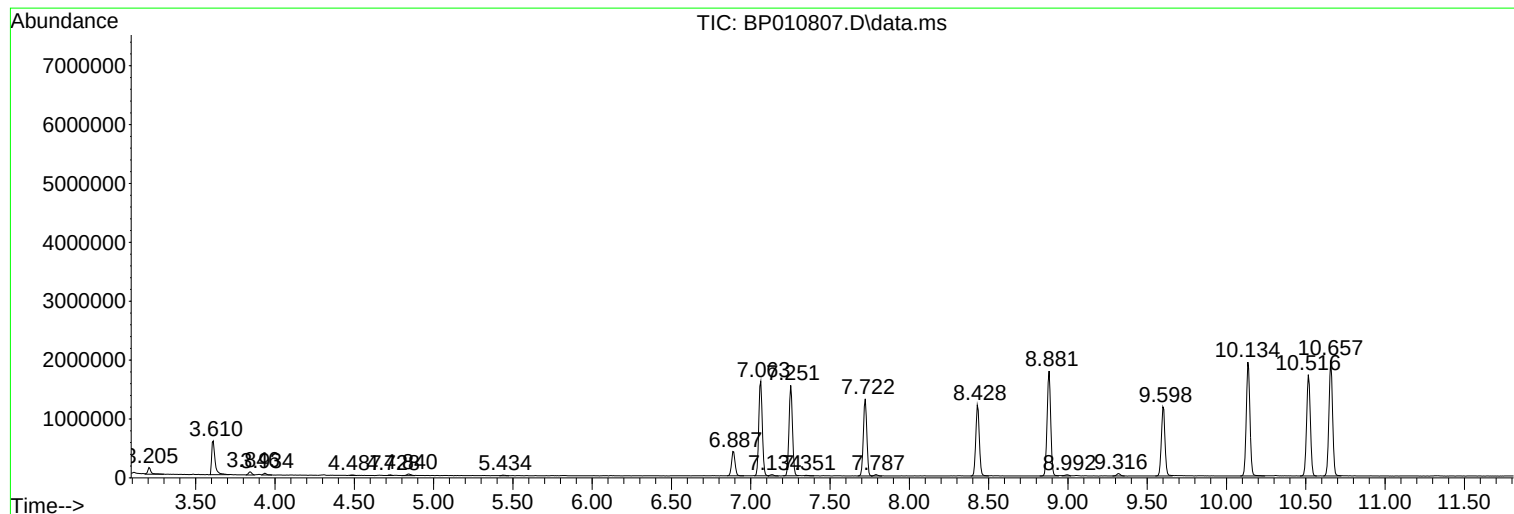

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010807.D
Acq On : 24 Jun 2022 22:55
Operator : CG/JU
Sample : N3401-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062422\
Data File : BP010807.D
Acq On : 24 Jun 2022 22:55
Operator : CG/JU
Sample : N3401-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
