
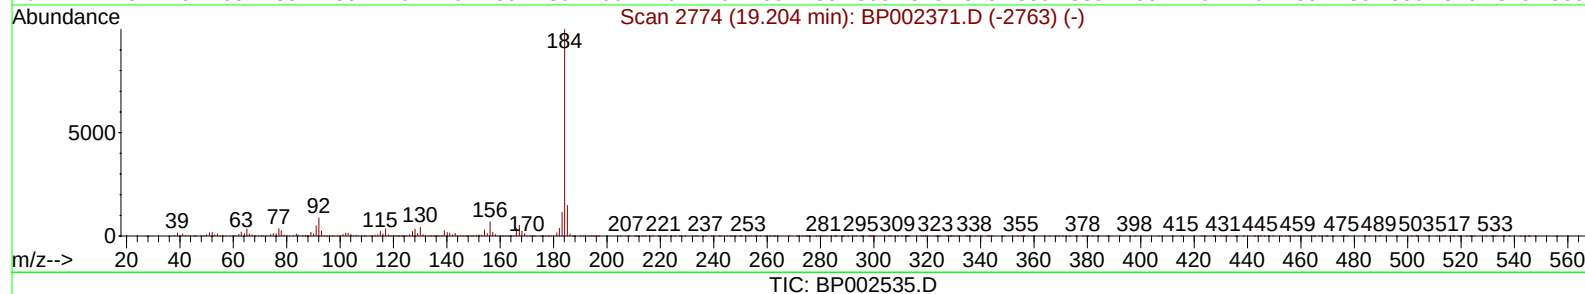
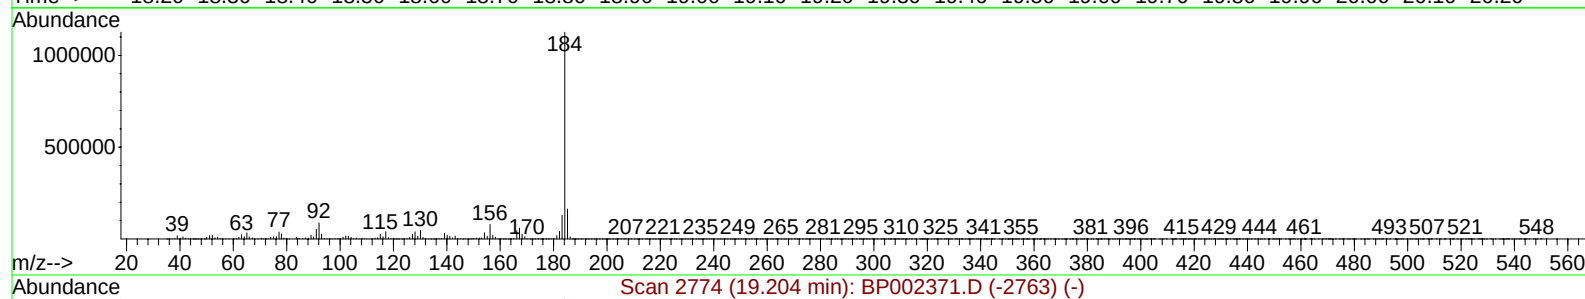


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062520\
 Data File : BP002535.D
 Acq On : 25 Jun 2020 09:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 17:34:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 24 13:54:06 2020
 Response via : Initial Calibration

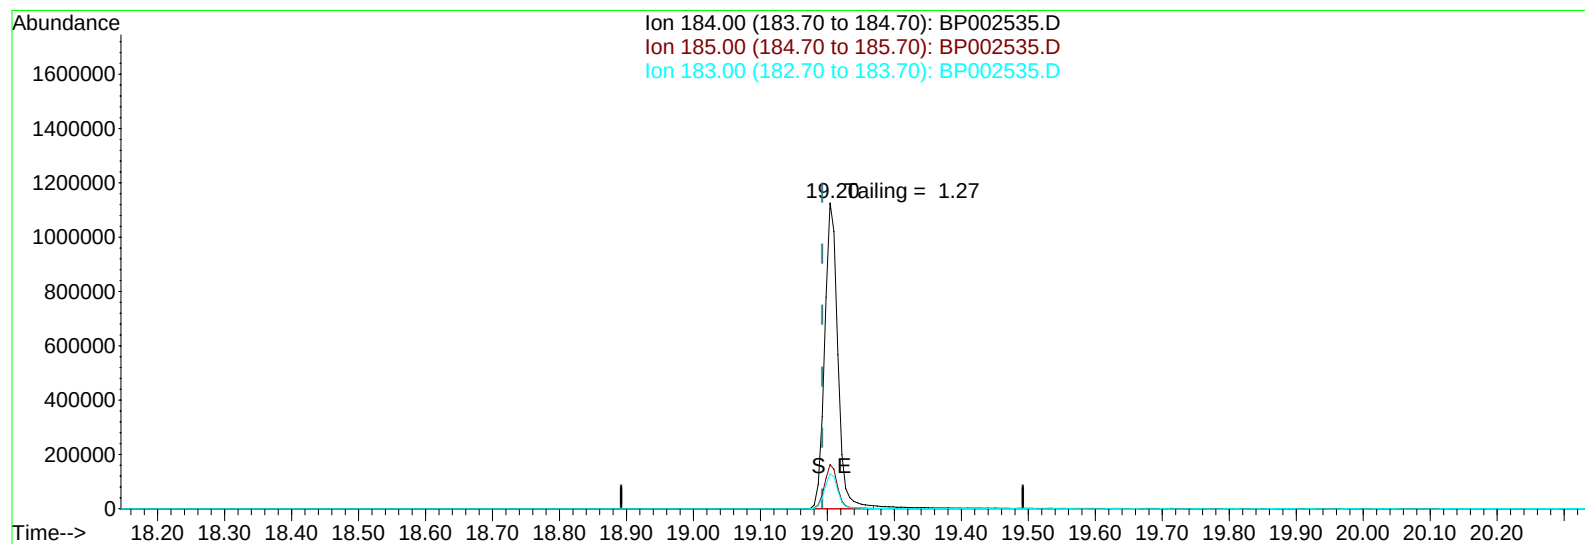

(77) Benzidine




19.204min (+0.012) 495469.71ng

response 1561051

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.46
183.00	11.50	11.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062520\
Data File : BP002535.D
Acq On : 25 Jun 2020 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 17:34:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 24 13:54:06 2020
Response via : Initial Calibration

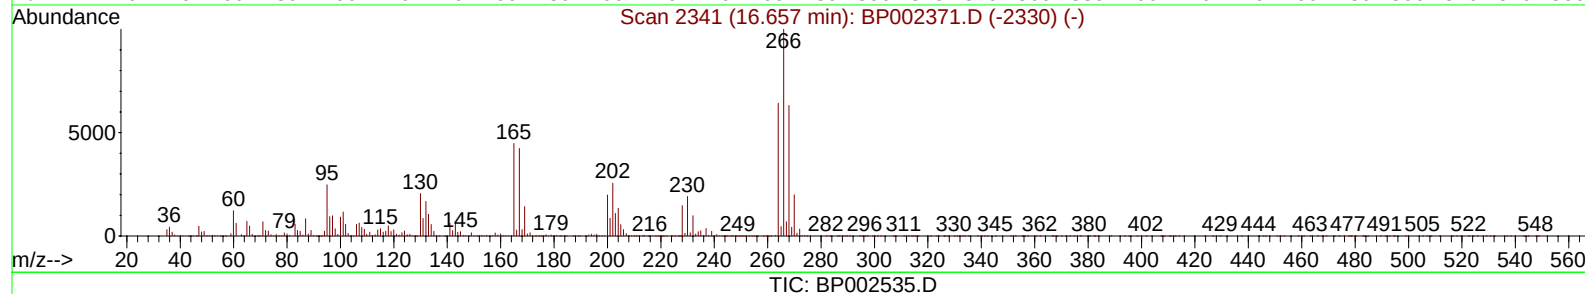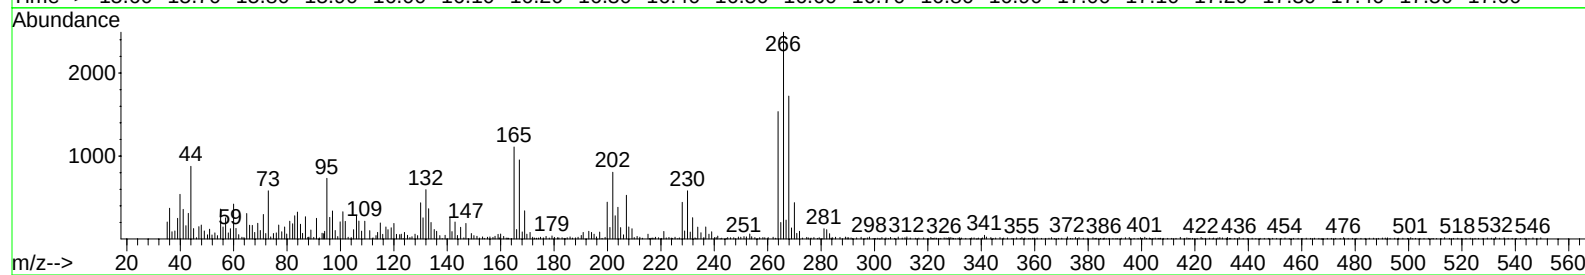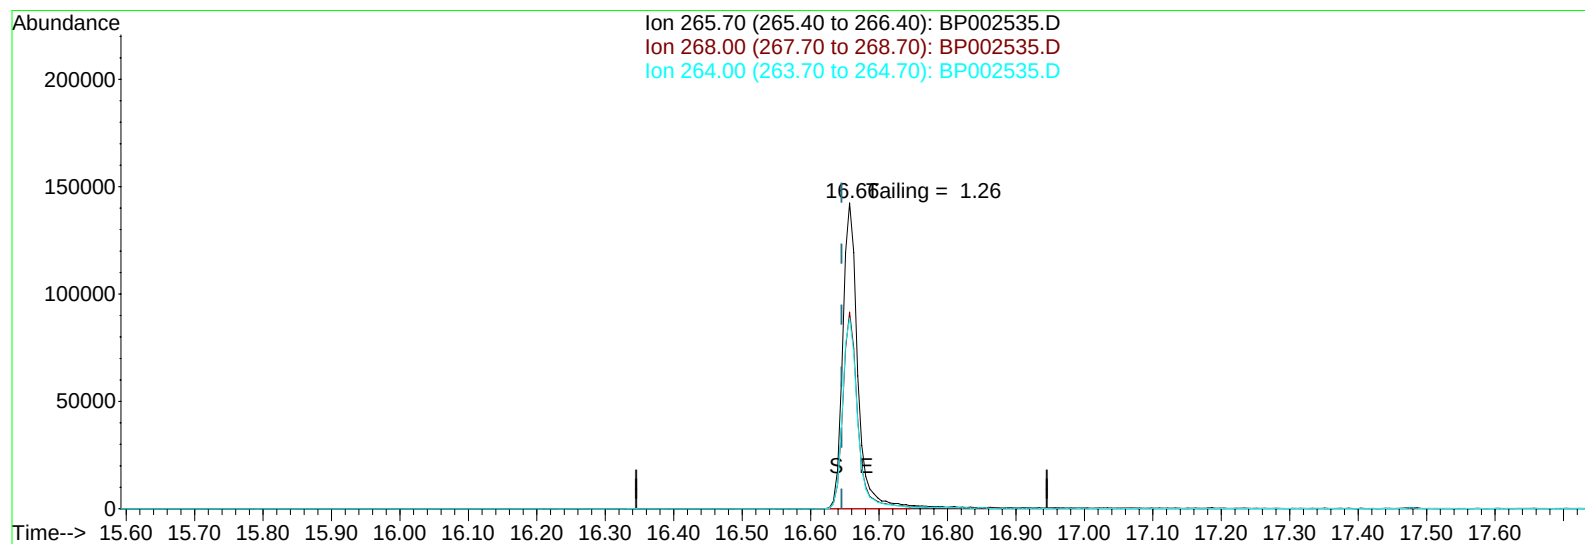

(70) Pentachlorophenol (C)

16.722min (+0.076) 2016.27ng m

response 1540

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	69.13
264.00	64.80	61.62
0.00	0.00	0.00