

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062520\
 Data File : BP002538.D
 Acq On : 25 Jun 2020 10:44
 Operator : CG/JU
 Sample : PB129731BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129731BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.205	387	394	413	rBV	3278226	5201613	44.50%	7.689%
2	6.781	649	662	689	rBV	3278177	5487098	46.94%	8.111%
3	7.581	791	798	809	rBV	789691	1279273	10.94%	1.891%
4	7.904	845	853	863	rBV	2925262	4862010	41.59%	7.187%
5	8.728	984	993	1016	rBV	2267692	3976519	34.02%	5.878%
6	10.357	1262	1270	1285	rBV	1032586	1773701	15.17%	2.622%
7	12.851	1686	1694	1718	rBV	5089565	8092068	69.23%	11.961%
8	14.234	1921	1929	1942	rBV2	1560136	2395364	20.49%	3.541%
9	15.733	2177	2184	2209	rBV	3914845	6323141	54.09%	9.347%
10	16.992	2389	2398	2410	rBV	1995458	2948146	25.22%	4.358%
11	19.586	2832	2839	2854	rBV	8147584	11689120	100.00%	17.278%
12	20.892	3057	3061	3070	rVV	302118	422485	3.61%	0.624%
13	21.098	3091	3096	3104	rBV2	2660634	3431870	29.36%	5.073%
14	21.704	3196	3199	3204	rVB	135603	154946	1.33%	0.229%
15	22.163	3273	3277	3282	rBV	295102	379217	3.24%	0.561%
16	22.668	3358	3363	3373	rVB	459149	663082	5.67%	0.980%
17	23.233	3453	3459	3464	rBV	573541	981767	8.40%	1.451%
18	23.298	3464	3470	3483	rVB	1911007	3645468	31.19%	5.389%
19	23.874	3562	3568	3580	rVB	567947	1078771	9.23%	1.595%
20	24.615	3688	3694	3707	rVB	515864	1143457	9.78%	1.690%
21	25.486	3835	3842	3859	rVB	361456	949773	8.13%	1.404%
22	26.509	4010	4016	4027	rVB	272864	772840	6.61%	1.142%




Sum of corrected areas: 67651729

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP062520\
Data File : BP002538.D
Acq On : 25 Jun 2020 10:44
Operator : CG/JU
Sample : PB129731BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129731BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

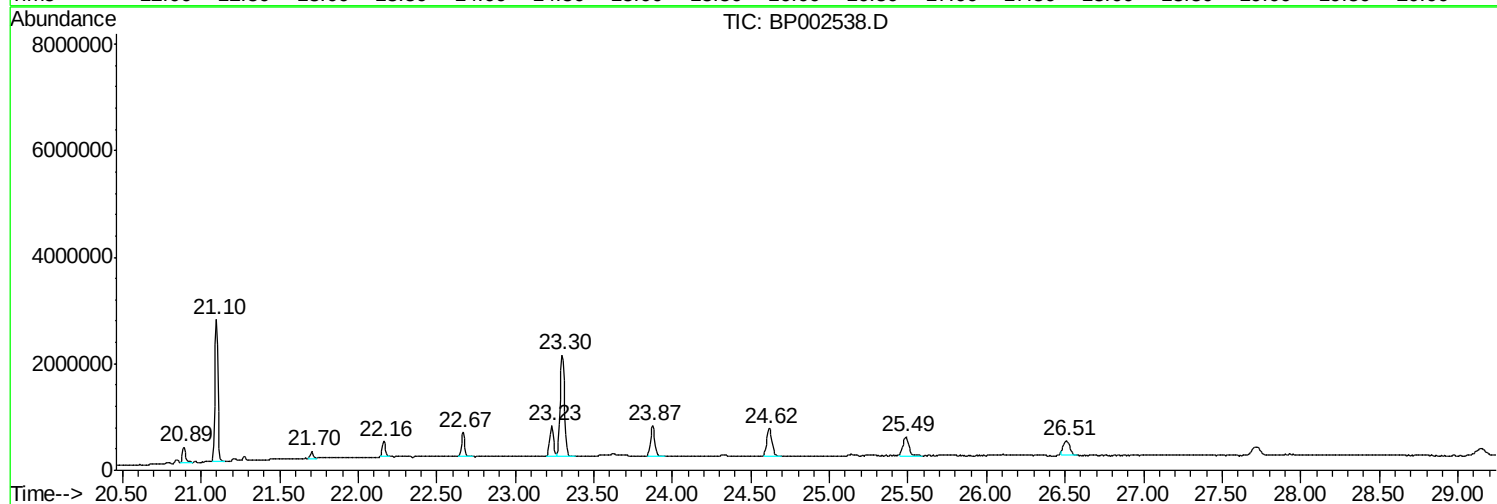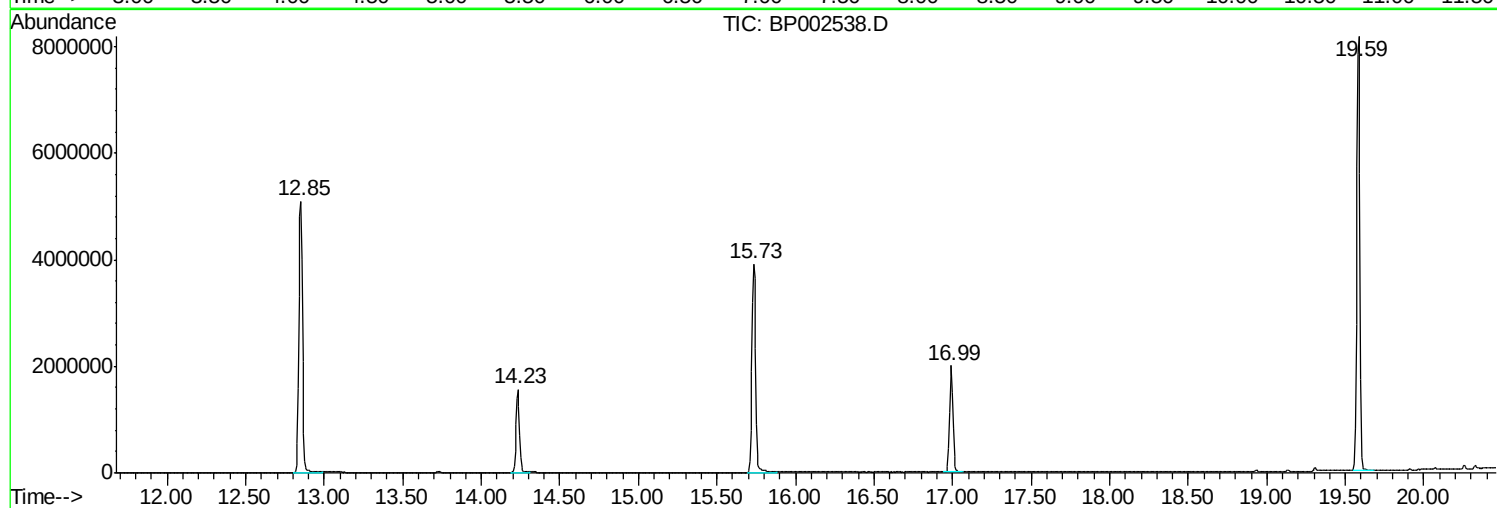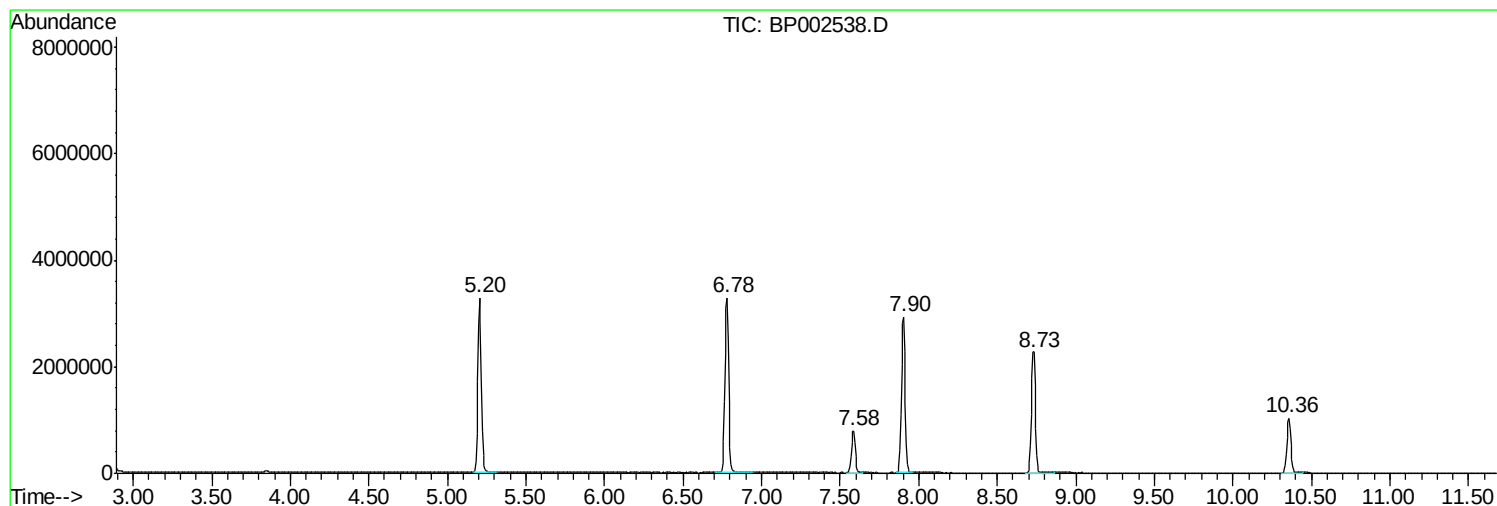

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP062520\
Data File : BP002538.D
Acq On : 25 Jun 2020 10:44
Operator : CG/JU
Sample : PB129731BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129731BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP062520\
Data File : BP002538.D
Acq On : 25 Jun 2020 10:44
Operator : CG/JU
Sample : PB129731BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129731BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc