


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062520\
 Data File : BP002535.D
 Acq On : 25 Jun 2020 09:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 24 13:54:06 2020

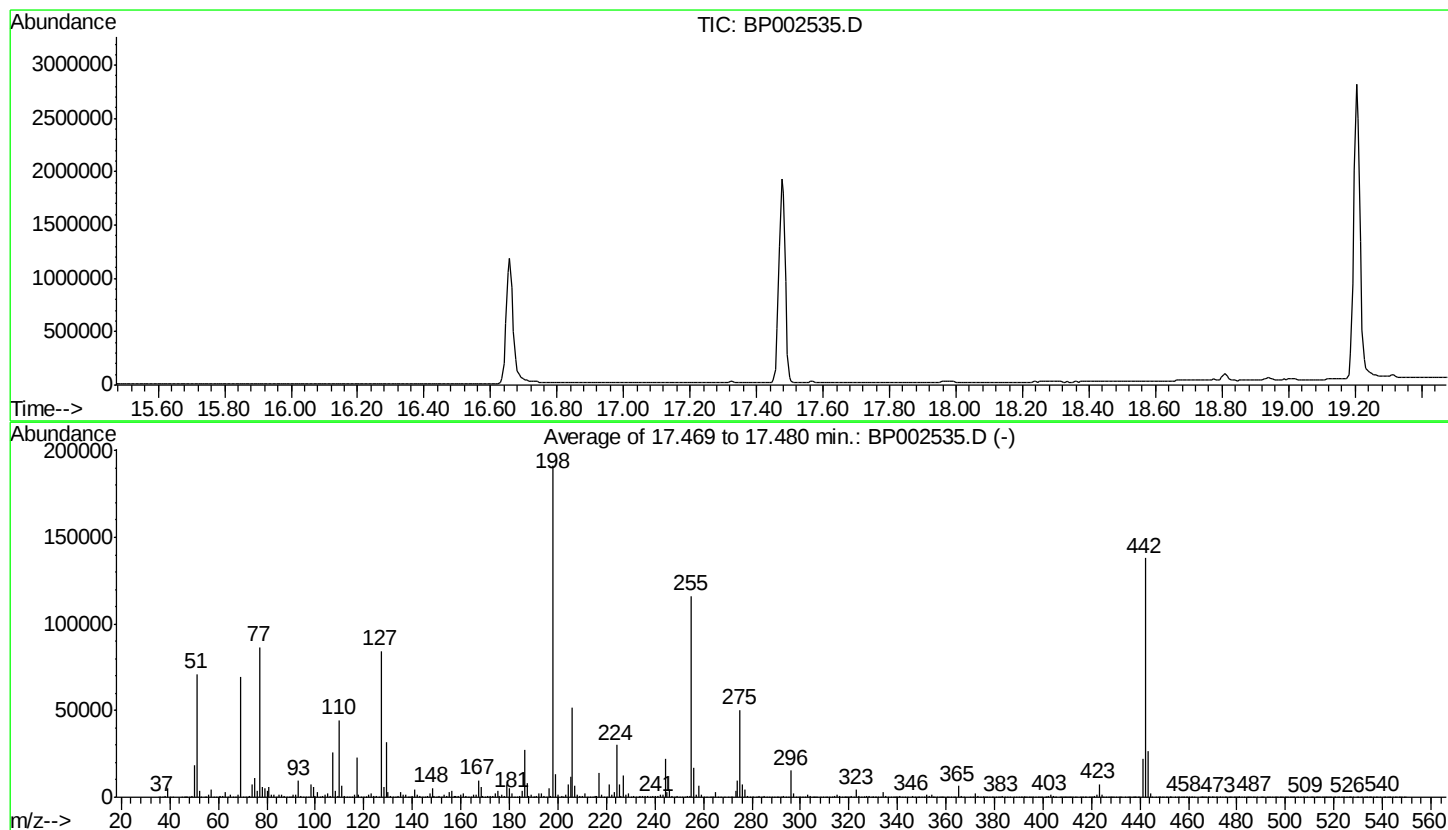

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	71182	PASS
68	69	0.00	2	1.8	1244	PASS
69	198	0.00	100	36.4	69637	PASS
70	69	0.00	2	0.5	351	PASS
127	198	10	80	44.1	84433	PASS
197	198	0.00	2	0.5	1004	PASS
198	198	100	100	100.0	191400	PASS
199	198	5	9	6.9	13151	PASS
275	198	10	60	26.3	50356	PASS
365	198	1	100	3.5	6632	PASS
441	198	0.01	100	11.6	22252	PASS
442	198	50	100	72.1	138007	PASS
443	442	15	24	19.0	26282	PASS