

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010845.D
 Acq On : 26 Jun 2022 01:11
 Operator : CG/JU
 Sample : N3392-15 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXEZ0

Quant Time: Jun 26 22:55:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 22:42:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	454784	20.000	ng/ul	0.00
20) Naphthalene-d8	10.510	136	1834740	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.369	164	968629	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.133	188	1829227	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.245	240	1791435	20.000	ng/ul	#-0.01
88) Perylene-d12	23.610	264	1879815	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	33871	2.817	ng/uL	0.00
4) Pyridine-d5	3.617	84	306608	9.581	ng/ul	0.01
7) Phenol-d5	6.893	99	317410	8.817	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.058	67	904141	38.402	ng/ul	0.00
11) 2-Chlorophenol-d4	7.252	132	926285	31.012	ng/ul	0.00
15) 4-Methylphenol-d8	8.434	113	574242	20.178	ng/ul	0.00
21) Nitrobenzene-d5	8.875	128	547960	46.915	ng/ul	0.00
24) 2-Nitrophenol-d4	9.599	143	504519	52.211	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.134	165	849827	35.593	ng/ul	0.00
31) 4-Chloroaniline-d4	10.657	131	1247295	32.003	ng/ul	0.00
46) Dimethylphthalate-d6	13.792	166	2752242	41.480	ng/ul	0.00
49) Acenaphthylene-d8	14.063	160	3334129	39.372	ng/ul	0.00
54) 4-Nitrophenol-d4	14.587	143	78277	7.553	ng/ul	0.00
60) Fluorene-d10	15.369	176	2340297	41.101	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.486	200	199044	32.843	ng/ul	-0.01
73) Anthracene-d10	17.233	188	3515038	43.190	ng/ul	-0.01
81) Pyrene-d10	19.480	212	3935678	40.325	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.457	264	4143487	44.605	ng/ul	-0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.540	105	45653	1.045	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010845.D
Acq On : 26 Jun 2022 01:11
Operator : CG/JU
Sample : N3392-15 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXEZ0

Quant Time: Jun 26 22:55:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 22:42:26 2022
Response via : Initial Calibration

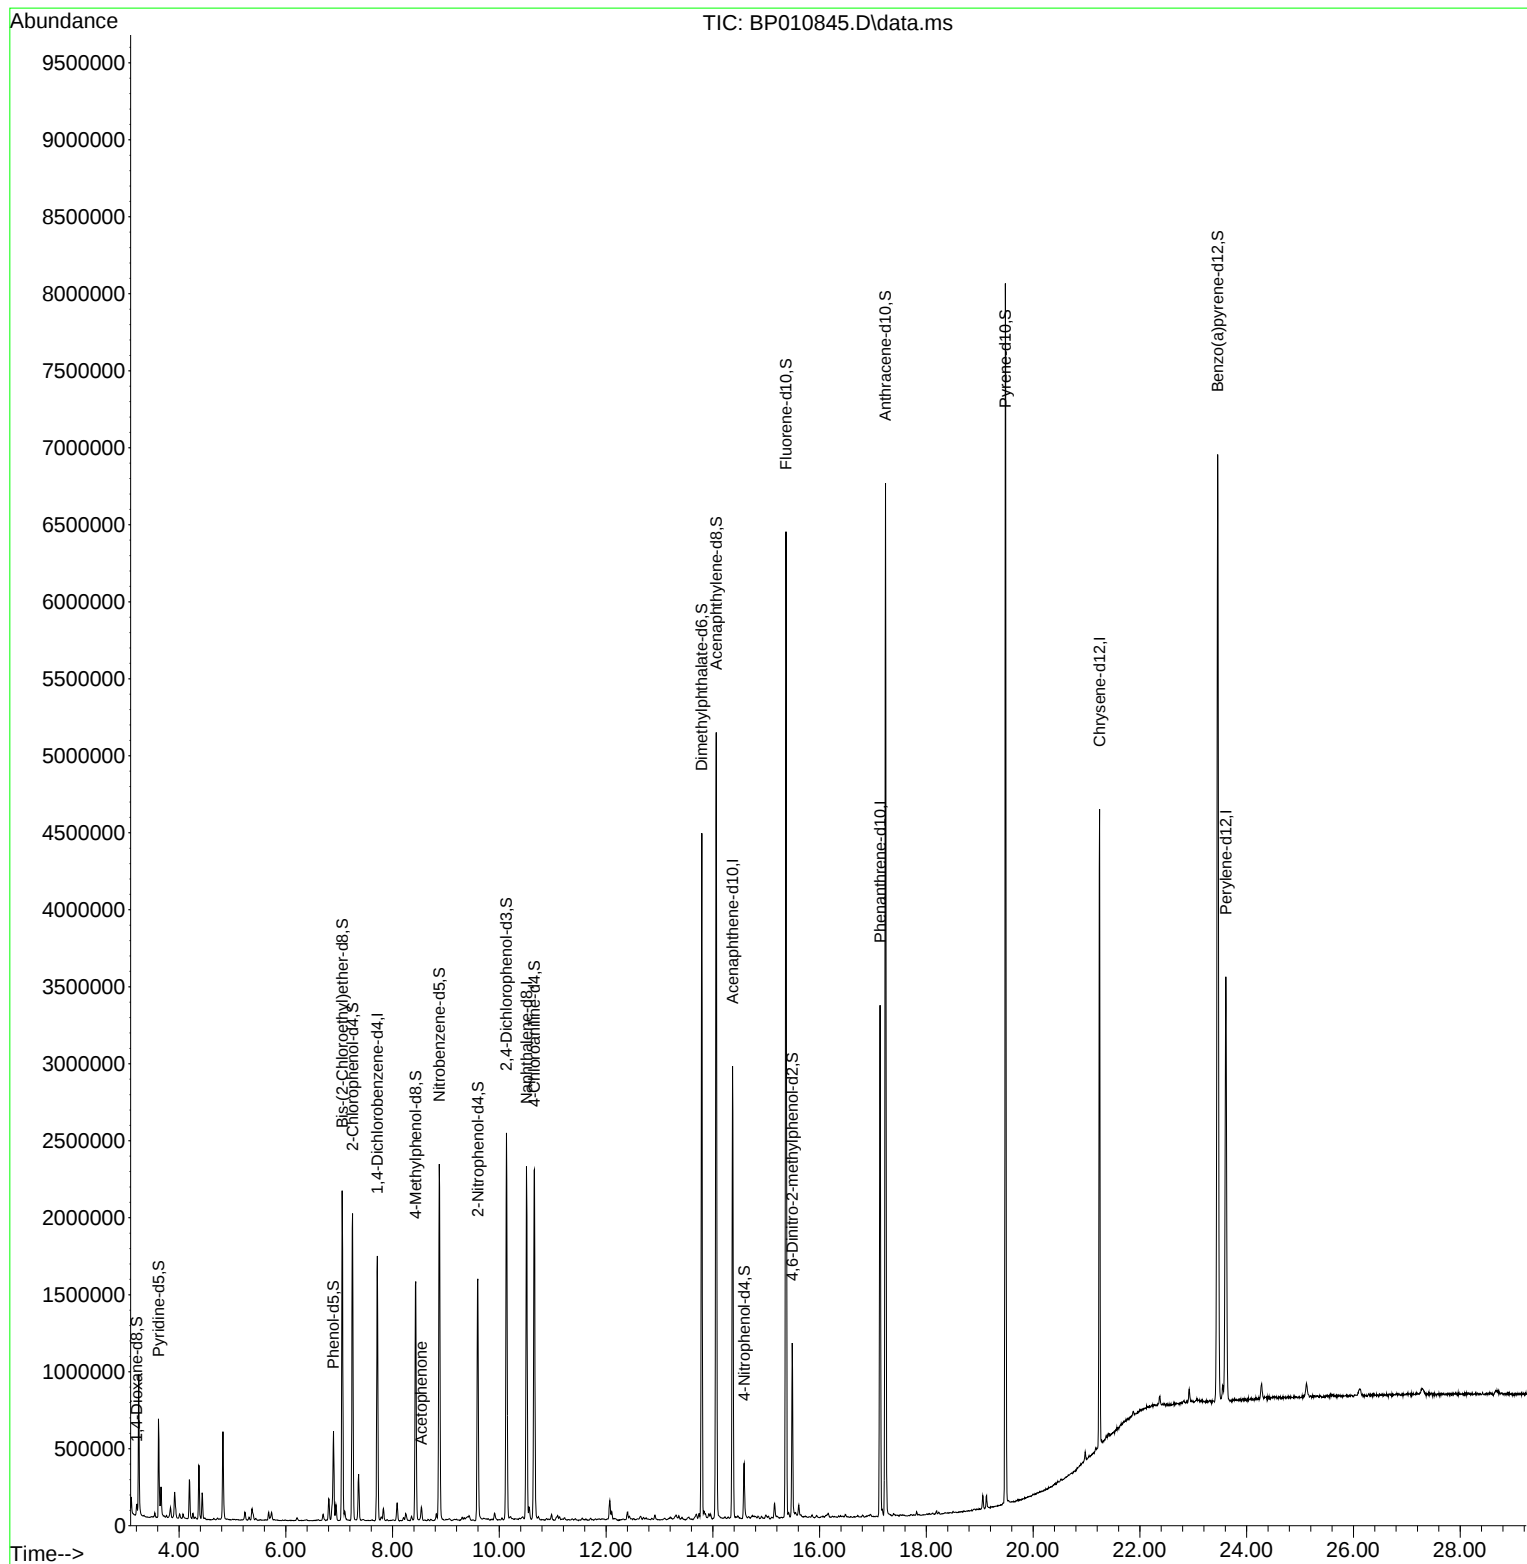

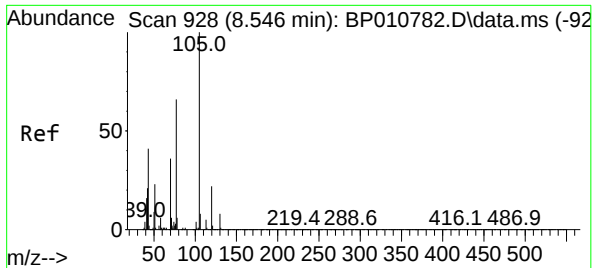

#16
 Acetophenone
 Concen: 1.045 ng/ul
 RT: 8.540 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP010845.D
 Acq: 26 Jun 2022 01:11

Instrument :
 BNA_P
 ClientSampleId :
 EXEZ0

Tgt Ion:	105	Resp:	45653
Ion Ratio	Lower	Upper	
105	100		
77	77.0	67.5	101.3
51	28.6	29.6	44.4#

