




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010826.D
 Acq On : 25 Jun 2022 13:55
 Operator : CG/JU
 Sample : N3355-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0C5

Manual IntegrationsAPPROVED

Quant Time: Jun 26 22:52:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 22:42:26 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :mohammad ahmed 07/01/2022

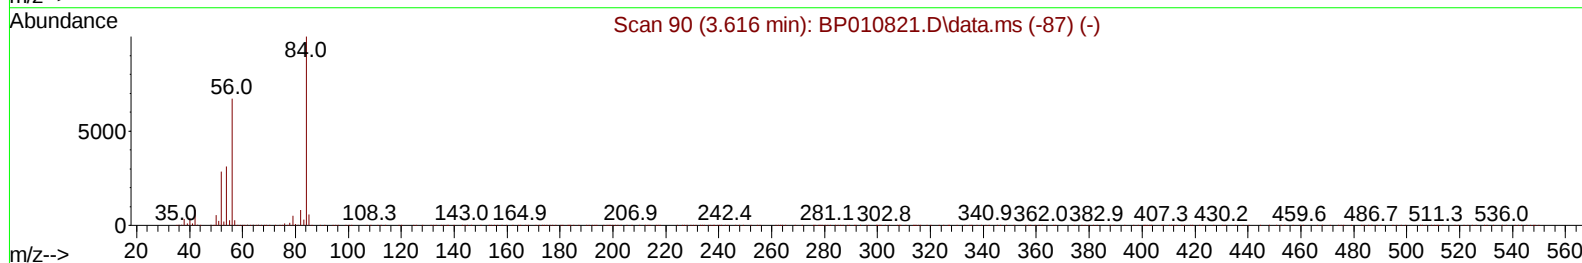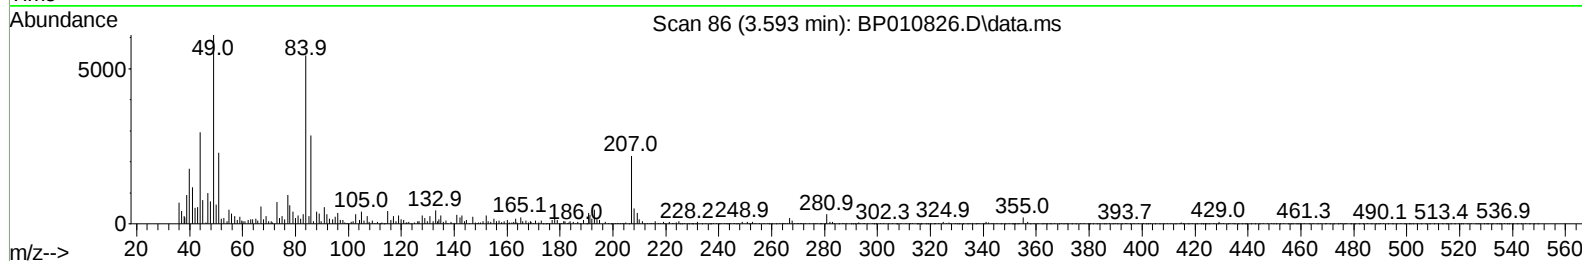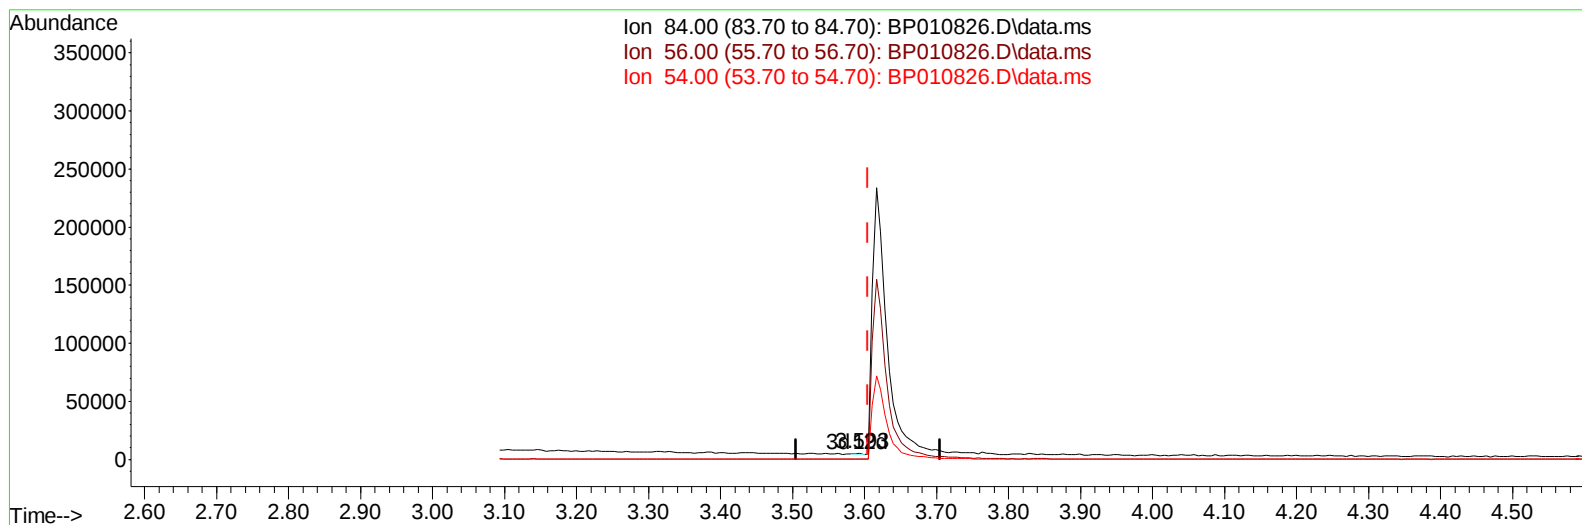

TIC: BP010826.D\data.ms

(4) Pyridine-d5 (S)

3.593min (-0.012) 0.02 ng/u1

response 557

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	84.50	6.00#
54.00	44.80	1.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010826.D
 Acq On : 25 Jun 2022 13:55
 Operator : CG/JU
 Sample : N3355-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0C5

Manual IntegrationsAPPROVED

Quant Time: Jun 26 22:52:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 22:42:26 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :mohammad ahmed 07/01/2022

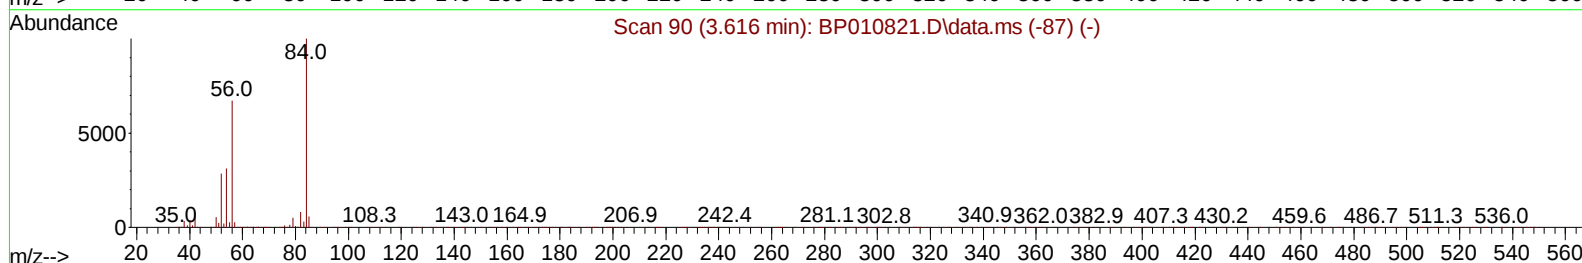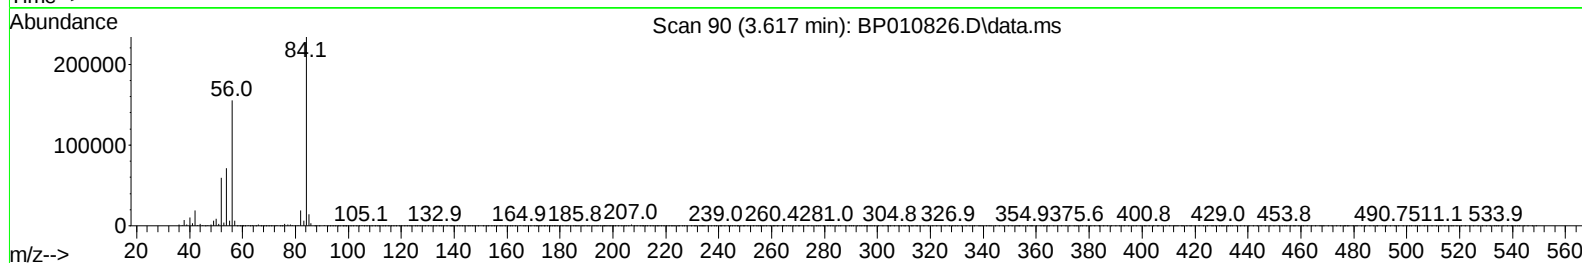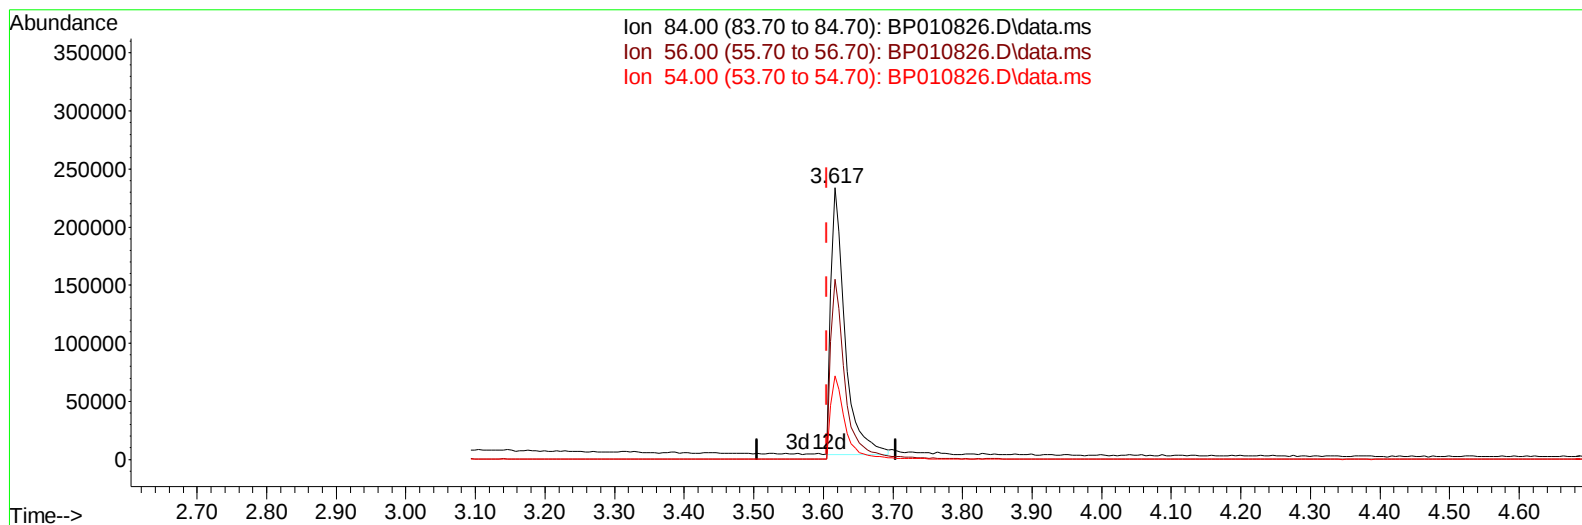

TIC: BP010826.D\data.ms

(4) Pyridine-d5 (S)

3.617min (+ 0.012) 9.04 ng/ul m

response 321881

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	84.50	66.44#
54.00	44.80	30.68#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010826.D
 Acq On : 25 Jun 2022 13:55
 Operator : CG/JU
 Sample : N3355-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0C5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :mohammad ahmed 07/01/2022

Quant Time: Jun 26 22:52:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 22:42:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	505835	20.000	ng/ul	0.00
20) Naphthalene-d8	10.516	136	2040541	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.375	164	1110227	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	2141861	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.251	240	2134066	20.000	ng/ul	# 0.00
88) Perylene-d12	23.621	264	2264431	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.211	96	26311	1.968	ng/uL	0.00
4) Pyridine-d5	3.617	84	321881m	9.043	ng/ul	0.01
7) Phenol-d5	6.899	99	260329	6.501	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	778396	29.724	ng/ul	0.00
11) 2-Chlorophenol-d4	7.252	132	794099	23.903	ng/ul	0.00
15) 4-Methylphenol-d8	8.440	113	488382	15.429	ng/ul	0.00
21) Nitrobenzene-d5	8.881	128	484435	37.293	ng/ul	0.00
24) 2-Nitrophenol-d4	9.599	143	454767	42.316	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.140	165	759111	28.587	ng/ul	0.00
31) 4-Chloroaniline-d4	10.663	131	1055724	24.356	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	2526083	33.216	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	3030381	31.221	ng/ul	0.00
54) 4-Nitrophenol-d4	14.592	143	68685	5.782	ng/ul	0.01
60) Fluorene-d10	15.375	176	2162890	33.141	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	194159	27.361	ng/ul	0.00
73) Anthracene-d10	17.239	188	3217141	33.760	ng/ul	0.00
81) Pyrene-d10	19.486	212	3694663	31.778	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.468	264	3843586	34.349	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010826.D
Acq On : 25 Jun 2022 13:55
Operator : CG/JU
Sample : N3355-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :mohammad ahmed 07/01/2022

Quant Time: Jun 26 22:52:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 22:42:26 2022
Response via : Initial Calibration

