

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010822.D
 Acq On : 25 Jun 2022 11:39
 Operator : CG/JU
 Sample : PB145658BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK658

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	17	21	28	rVB	162173	198773	2.27%	0.205%
2	3.617	86	90	114	rBV	1941689	2715567	31.02%	2.797%
3	3.934	140	144	151	rVB	33498	49386	0.56%	0.051%
4	6.905	639	649	663	rBV	2007303	3099419	35.40%	3.192%
5	7.064	667	676	687	rVB	1686065	2607686	29.78%	2.686%
6	7.258	702	709	717	rBV	2128483	3264171	37.28%	3.362%
7	7.722	781	788	799	rVB	1670082	2569103	29.34%	2.646%
8	8.446	903	911	919	rBV	2489871	3819155	43.62%	3.934%
9	8.887	976	986	997	rBV	1818923	2938806	33.57%	3.027%
10	9.605	1100	1108	1117	rBV	1423340	2194632	25.07%	2.260%
11	10.146	1192	1200	1216	rBV	2218615	3534493	40.37%	3.640%
12	10.522	1256	1264	1272	rVB	2118586	3557612	40.63%	3.664%
13	10.663	1280	1288	1305	rBV	2323643	3803540	43.44%	3.917%
14	12.116	1528	1535	1542	rVB	43719	75283	0.86%	0.078%
15	12.328	1567	1571	1580	rVB10	6504	13565	0.15%	0.014%
16	13.346	1740	1744	1748	rBV4	6362	8767	0.10%	0.009%
17	13.798	1815	1821	1835	rBV	3315025	4658990	53.21%	4.799%
18	14.069	1860	1867	1877	rBV	3974327	5855648	66.88%	6.031%
19	14.381	1913	1920	1929	rBV	2809353	4129183	47.16%	4.253%
20	14.598	1950	1957	1971	rBV	1400365	2080759	23.77%	2.143%
21	14.804	1990	1992	2000	rVB9	6262	11631	0.13%	0.012%
22	15.198	2057	2059	2066	rVB8	5125	9523	0.11%	0.010%
23	15.381	2083	2090	2101	rBV	4986227	6962351	79.52%	7.171%
24	15.498	2104	2110	2125	rBV	870757	1231076	14.06%	1.268%
25	15.622	2126	2131	2135	rVB	55449	88661	1.01%	0.091%
26	16.169	2220	2224	2230	rBV7	16442	24683	0.28%	0.025%
27	16.822	2331	2335	2339	rBV6	9662	14998	0.17%	0.015%
28	16.928	2349	2353	2354	rBV4	6685	8827	0.10%	0.009%
29	17.145	2383	2390	2396	rBV	3100237	4279551	48.88%	4.408%
30	17.245	2400	2407	2417	rBV	5035134	7061430	80.65%	7.273%
31	17.404	2429	2434	2439	rBV7	12481	18096	0.21%	0.019%
32	19.069	2713	2717	2722	rBV	65239	84175	0.96%	0.087%
33	19.133	2725	2728	2732	rVV2	56352	70935	0.81%	0.073%
34	19.492	2783	2789	2796	rBV	6074909	7817699	89.29%	8.052%
35	21.251	3084	3088	3093	rBV	3689621	4570261	52.20%	4.707%
36	23.474	3459	3466	3475	rVB2	4472520	8755534	100.00%	9.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010822.D
Acq On : 25 Jun 2022 11:39
Operator : CG/JU
Sample : PB145658BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK658

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION

37 23.627 3486 3492 3500 rVB2 2454860 4907364 56.05% 5.054%




Sum of corrected areas: 97091333

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010822.D
Acq On : 25 Jun 2022 11:39
Operator : CG/JU
Sample : PB145658BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK658

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

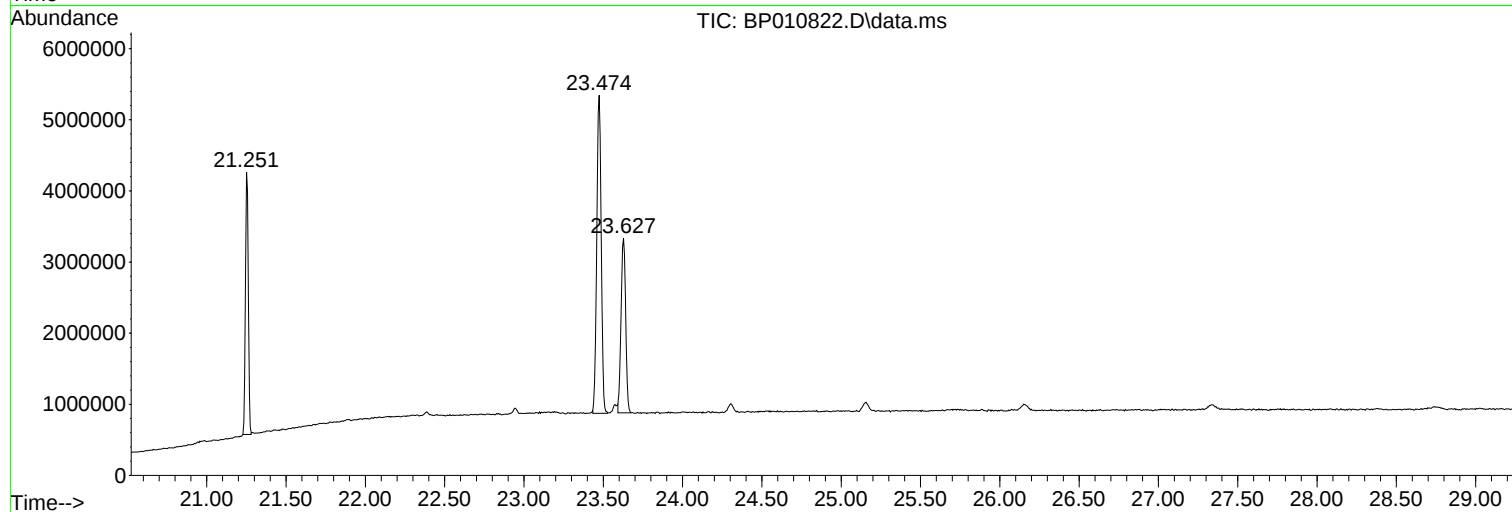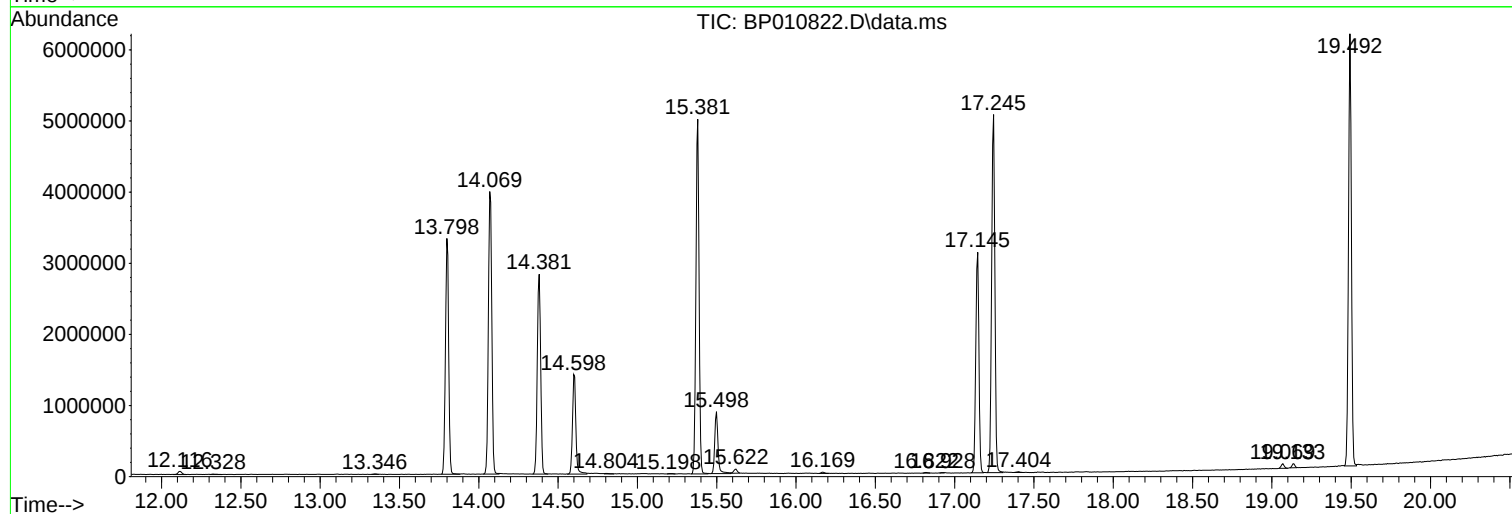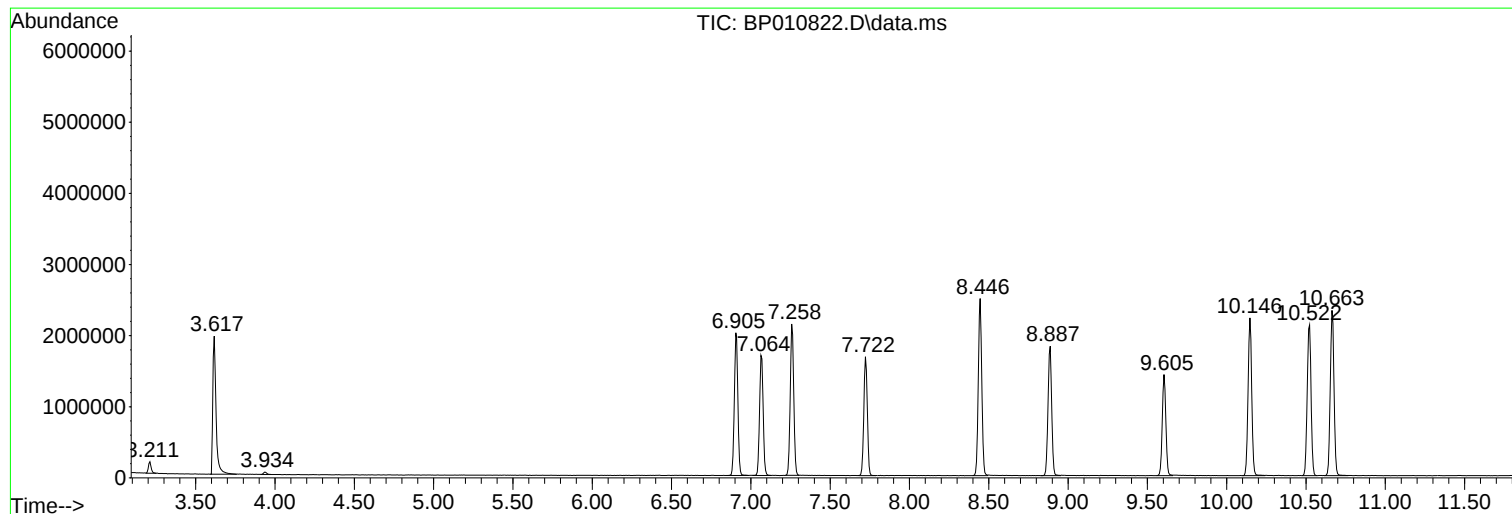

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010822.D
Acq On : 25 Jun 2022 11:39
Operator : CG/JU
Sample : PB145658BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK658

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010822.D
Acq On : 25 Jun 2022 11:39
Operator : CG/JU
Sample : PB145658BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK658

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------