

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010825.D
 Acq On : 25 Jun 2022 13:21
 Operator : CG/JU
 Sample : PB145664BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	32	rVB	168350	227970	2.59%	0.235%
2	3.616	86	90	109	rBV	1992693	2907186	32.99%	2.994%
3	3.934	140	144	151	rVB	35436	52586	0.60%	0.054%
4	6.904	639	649	657	rBV	2070720	3210205	36.43%	3.306%
5	7.063	669	676	686	rVB	1828541	2752417	31.24%	2.835%
6	7.257	701	709	718	rBV	2176768	3427769	38.90%	3.530%
7	7.722	780	788	794	rBV	1483244	2342535	26.59%	2.413%
8	8.440	902	910	922	rBV	2630372	4024946	45.68%	4.145%
9	8.881	978	985	993	rBV	1971987	3098562	35.17%	3.191%
10	9.598	1098	1107	1122	rBV	1434504	2319339	26.32%	2.389%
11	10.139	1192	1199	1212	rBV	2282148	3679964	41.76%	3.790%
12	10.516	1254	1263	1275	rVB	2044587	3273180	37.15%	3.371%
13	10.663	1278	1288	1298	rBV	2399417	4017780	45.60%	4.138%
14	12.110	1529	1534	1540	rVB	47015	75203	0.85%	0.077%
15	12.328	1563	1571	1575	rVB	6136	11745	0.13%	0.012%
16	13.345	1738	1744	1747	rVB5	6590	9393	0.11%	0.010%
17	13.798	1814	1821	1828	rBV	3448050	4840099	54.93%	4.985%
18	14.069	1857	1867	1879	rBV	4174530	6129617	69.57%	6.313%
19	14.375	1913	1919	1926	rBV	2638930	3778003	42.88%	3.891%
20	14.592	1948	1956	1971	rBV	1411217	2077471	23.58%	2.140%
21	15.210	2055	2061	2067	rBV	3840	10251	0.12%	0.011%
22	15.375	2082	2089	2101	rBV	5301260	7226711	82.02%	7.443%
23	15.492	2102	2109	2122	rVV	893404	1229769	13.96%	1.267%
24	15.616	2125	2130	2137	rVB2	63007	101332	1.15%	0.104%
25	16.163	2219	2223	2227	rBV3	19588	26672	0.30%	0.027%
26	16.810	2329	2333	2338	rBV8	12888	21455	0.24%	0.022%
27	16.916	2349	2351	2356	rBV6	7414	10856	0.12%	0.011%
28	17.139	2382	2389	2398	rVV	2713667	3832346	43.49%	3.947%
29	17.239	2399	2406	2419	rVV	5201865	7144092	81.08%	7.358%
30	17.398	2430	2433	2438	rVB7	10766	17535	0.20%	0.018%
31	19.063	2712	2716	2721	rVB2	65151	84539	0.96%	0.087%
32	19.133	2724	2728	2734	rBV	64972	86115	0.98%	0.089%
33	19.486	2783	2788	2795	rBV	5800596	7693783	87.32%	7.924%
34	21.251	3083	3088	3094	rBV	3322581	4058602	46.06%	4.180%
35	23.468	3458	3465	3476	rVB2	4559526	8811129	100.00%	9.075%
36	23.621	3485	3491	3502	rVB2	2320855	4480984	50.86%	4.615%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010825.D
Acq On : 25 Jun 2022 13:21
Operator : CG/JU
Sample : PB145664BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK664

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 97092141

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010825.D
Acq On : 25 Jun 2022 13:21
Operator : CG/JU
Sample : PB145664BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK664

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

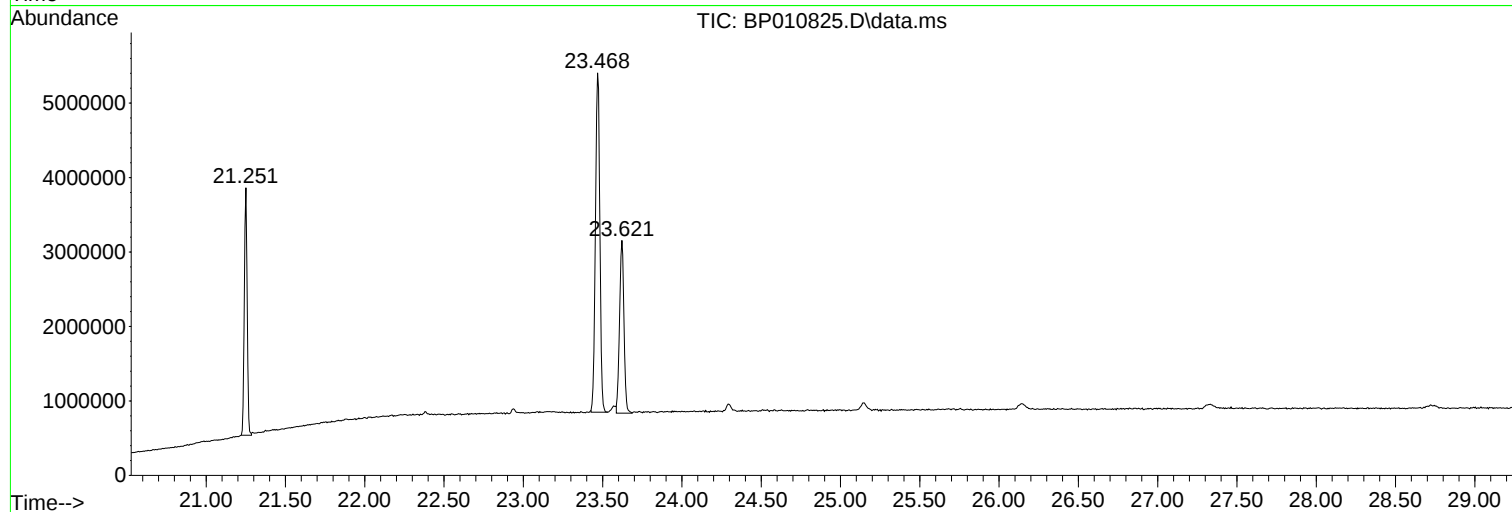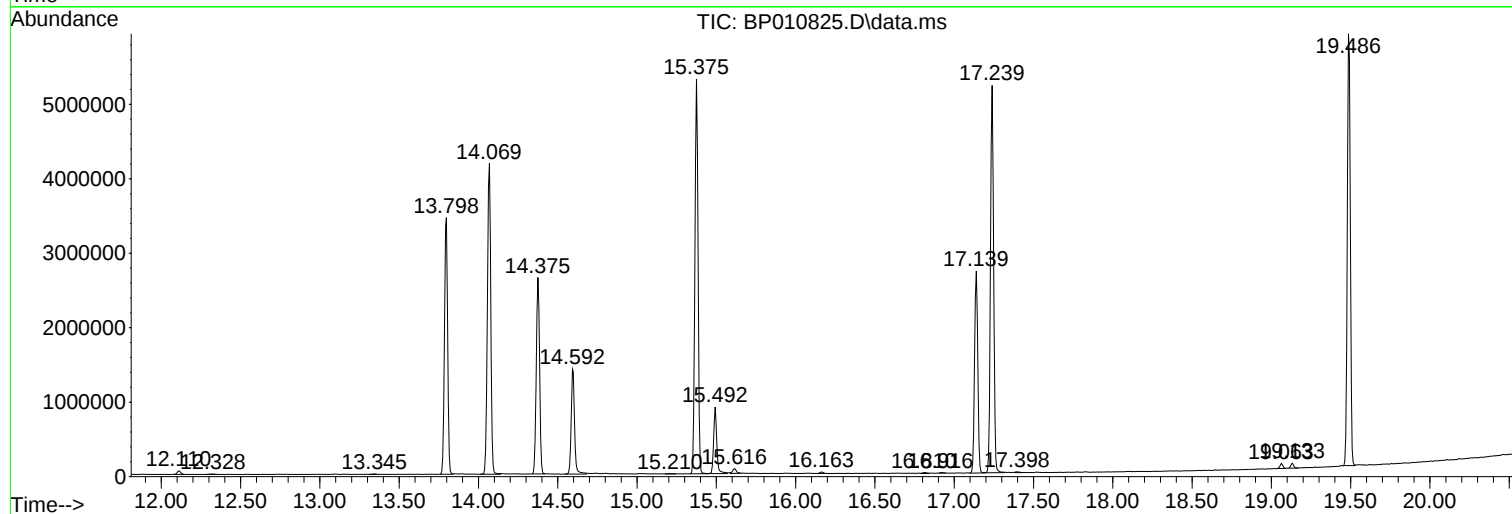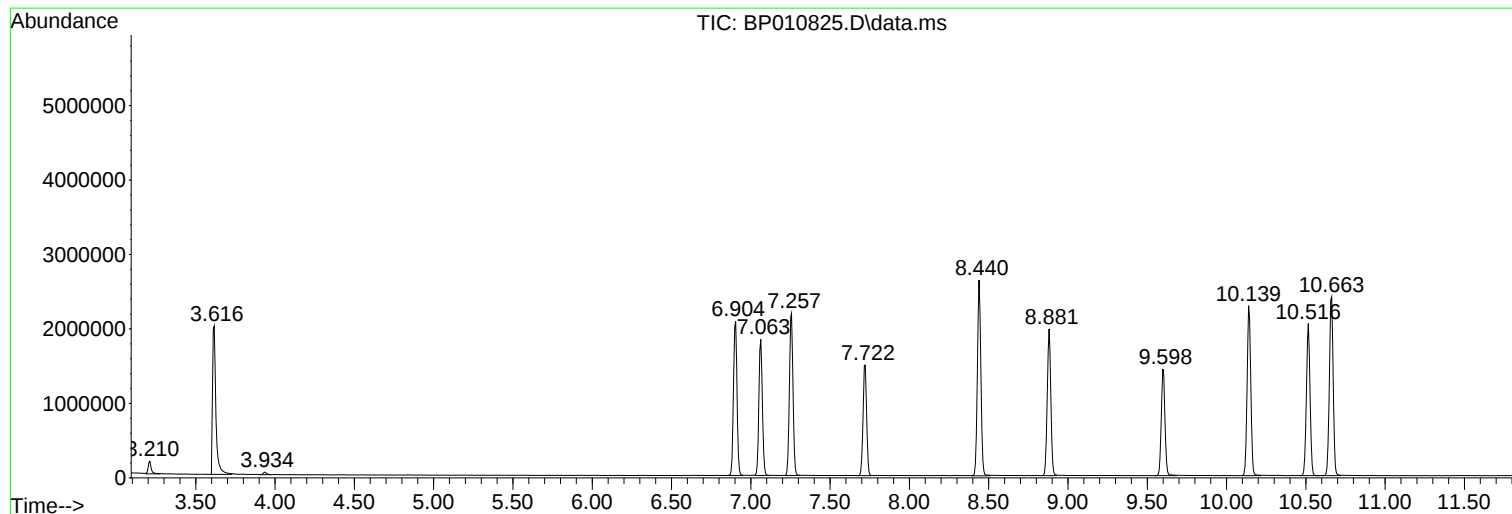

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010825.D
Acq On : 25 Jun 2022 13:21
Operator : CG/JU
Sample : PB145664BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK664

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010825.D
Acq On : 25 Jun 2022 13:21
Operator : CG/JU
Sample : PB145664BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK664

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc