

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010826.D
 Acq On : 25 Jun 2022 13:55
 Operator : CG/JU
 Sample : N3355-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0C5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	17	21	30	rVB	60260	85972	0.79%	0.082%
2	3.481	64	67	82	rVB	63533	102010	0.93%	0.098%
3	3.617	88	90	107	rBV	624789	890735	8.16%	0.852%
4	3.846	123	129	133	rBV	53279	82753	0.76%	0.079%
5	3.934	140	144	150	rVB	46511	63371	0.58%	0.061%
6	4.487	235	238	243	rVB4	11129	17574	0.16%	0.017%
7	4.728	274	279	282	rBV2	11914	15909	0.15%	0.015%
8	4.858	294	301	314	rBV2	182140	301186	2.76%	0.288%
9	5.440	396	400	408	rBV2	15886	23059	0.21%	0.022%
10	5.816	460	464	469	rVB2	8659	11365	0.10%	0.011%
11	6.899	640	648	656	rBV	461925	706400	6.47%	0.676%
12	7.063	666	676	683	rBV	1786388	2781769	25.47%	2.661%
13	7.134	683	688	695	rVB	55915	87792	0.80%	0.084%
14	7.252	702	708	718	rBV	1692524	2662811	24.38%	2.548%
15	7.346	719	724	731	rVB7	13527	23942	0.22%	0.023%
16	7.716	780	787	796	rBV	1874109	2944033	26.96%	2.817%
17	7.793	796	800	806	rVB2	17201	26981	0.25%	0.026%
18	8.440	901	910	921	rBV	1325048	2053124	18.80%	1.964%
19	8.881	977	985	993	rBV	1993158	3175214	29.07%	3.038%
20	9.052	1011	1014	1020	rVB6	10231	14762	0.14%	0.014%
21	9.310	1053	1058	1064	rVB	15266	25107	0.23%	0.024%
22	9.599	1098	1107	1122	rBV	1435399	2299575	21.05%	2.200%
23	10.140	1190	1199	1213	rBV	2185525	3517173	32.20%	3.365%
24	10.516	1255	1263	1271	rBV	2543687	4106644	37.60%	3.929%
25	10.663	1275	1288	1302	rBV	1924275	3279491	30.03%	3.138%
26	11.816	1476	1484	1489	rBV2	11027	19477	0.18%	0.019%
27	12.110	1528	1534	1541	rVB	48525	78432	0.72%	0.075%
28	13.210	1717	1721	1729	rVB3	14456	24306	0.22%	0.023%
29	13.345	1739	1744	1750	rBV4	17120	23107	0.21%	0.022%
30	13.798	1814	1821	1828	rBV	3945425	5371598	49.18%	5.139%
31	14.069	1858	1867	1879	rBV	4484862	6647468	60.86%	6.360%
32	14.287	1900	1904	1908	rVB3	10597	15280	0.14%	0.015%
33	14.375	1912	1919	1926	rBV	3364132	4863819	44.53%	4.653%
34	14.592	1950	1956	1965	rBV	326501	476828	4.37%	0.456%
35	14.739	1977	1981	1985	rBV6	7608	10925	0.10%	0.010%
36	14.810	1988	1993	1999	rVB8	15666	27070	0.25%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010826.D
 Acq On : 25 Jun 2022 13:55
 Operator : CG/JU
 Sample : N3355-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0C5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	15.163	2050	2053	2056	rBV5	7711	10988	0.10%	0.011%
38	15.198	2056	2059	2064	rVV4	8994	16079	0.15%	0.015%
39	15.245	2064	2067	2072	rVB6	12315	15440	0.14%	0.015%
40	15.375	2082	2089	2096	rBV	5996345	8236184	75.41%	7.880%
41	15.492	2103	2109	2124	rBV	1115782	1517695	13.90%	1.452%
42	15.616	2125	2130	2136	rVB2	66561	99851	0.91%	0.096%
43	16.163	2219	2223	2232	rVB5	25198	41547	0.38%	0.040%
44	16.810	2331	2333	2338	rVB5	9530	13566	0.12%	0.013%
45	16.916	2347	2351	2356	rBV3	32416	46544	0.43%	0.045%
46	17.139	2382	2389	2399	rBV	3870108	5344060	48.93%	5.113%
47	17.239	2399	2406	2418	rVV	6178272	8506036	77.88%	8.138%
48	17.339	2420	2423	2428	rVV5	21256	29109	0.27%	0.028%
49	17.392	2429	2432	2437	rVB5	12962	18229	0.17%	0.017%
50	17.833	2504	2507	2511	rVB4	19245	24824	0.23%	0.024%
51	19.063	2712	2716	2721	rBV2	82378	110204	1.01%	0.105%
52	19.133	2724	2728	2732	rVB	78297	99090	0.91%	0.095%
53	19.486	2782	2788	2796	rBV	7727237	9912163	90.76%	9.484%
54	20.980	3039	3042	3047	rBV	221869	243618	2.23%	0.233%
55	21.251	3083	3088	3094	rBV	4727385	6053464	55.43%	5.792%
56	23.468	3458	3465	3476	rVB2	5609676	10921803	100.00%	10.449%
57	23.621	3484	3491	3499	rVB2	3207586	6402440	58.62%	6.126%




Sum of corrected areas: 104519996

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010826.D
Acq On : 25 Jun 2022 13:55
Operator : CG/JU
Sample : N3355-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

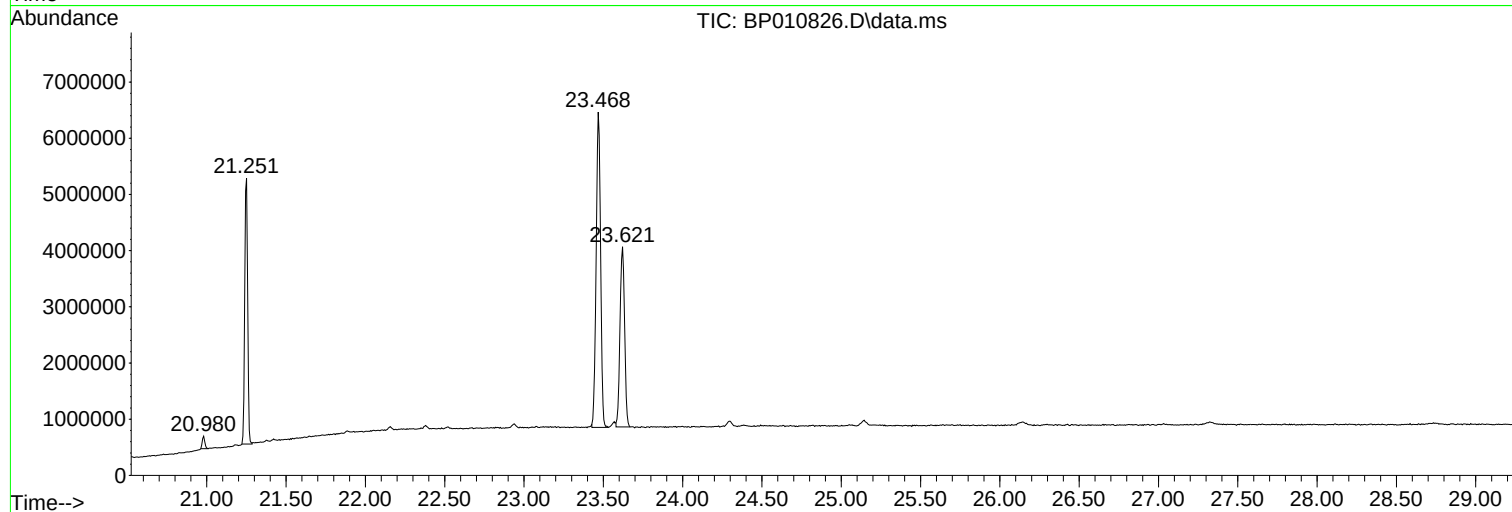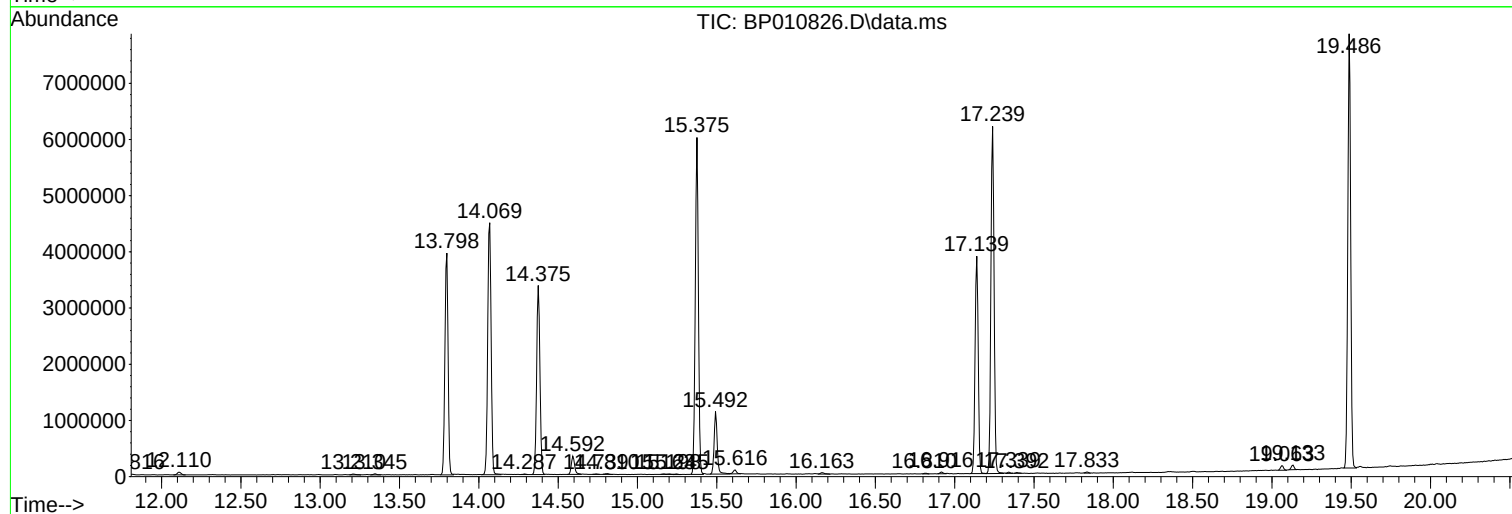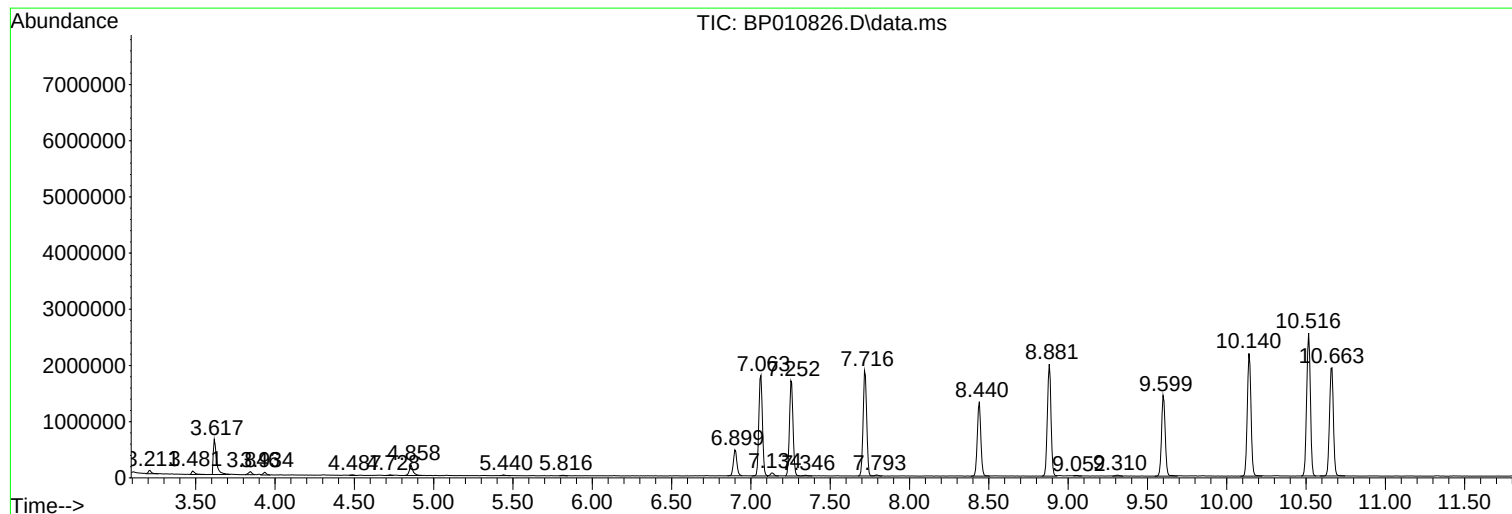

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010826.D
Acq On : 25 Jun 2022 13:55
Operator : CG/JU
Sample : N3355-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
4.858	2.05 ng/ul	301186	1,4-Dichlorobenzene-d4			7.716

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50	
2	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	47	
3	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40	
4	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	32	
5	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17	

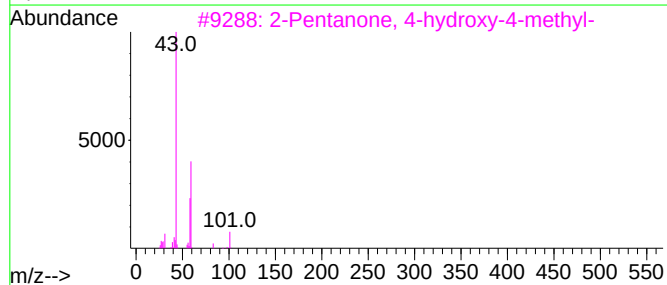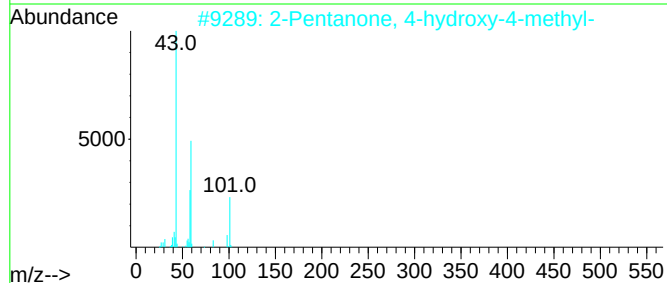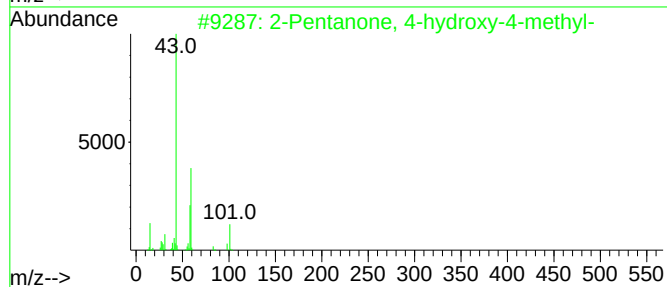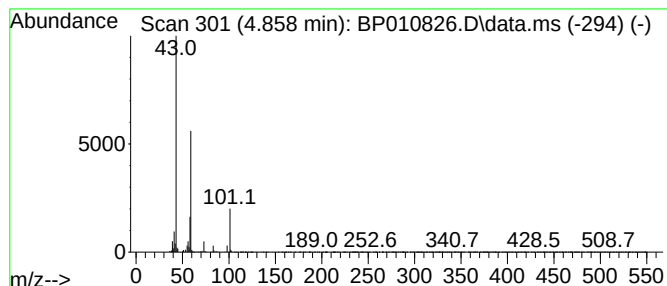

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010826.D
Acq On : 25 Jun 2022 13:55
Operator : CG/JU
Sample : N3355-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.858	2.0	ng/ul	301186	1	7.716	2944030	20.0