

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010827.D
 Acq On : 25 Jun 2022 14:29
 Operator : CG/JU
 Sample : N3355-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0D2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	17	21	28	rVB	62640	77057	0.86%	0.083%
2	3.552	74	79	84	rVB8	7193	9898	0.11%	0.011%
3	3.617	87	90	109	rBV	393796	594888	6.64%	0.643%
4	3.846	123	129	135	rVV	53955	82325	0.92%	0.089%
5	3.893	135	137	140	rVV3	7554	9259	0.10%	0.010%
6	3.934	140	144	148	rVB	37759	46064	0.51%	0.050%
7	4.064	163	166	170	rBV2	8222	10677	0.12%	0.012%
8	4.299	201	206	211	rBV4	22218	30941	0.35%	0.033%
9	4.440	227	230	234	rBV6	7704	10039	0.11%	0.011%
10	4.487	234	238	243	rVB2	9956	14478	0.16%	0.016%
11	4.728	274	279	282	rBV5	9480	17881	0.20%	0.019%
12	4.858	293	301	309	rBV2	138333	218653	2.44%	0.236%
13	5.275	368	372	377	rBV	24556	36199	0.40%	0.039%
14	5.316	377	379	385	rVB3	7225	10149	0.11%	0.011%
15	5.446	396	401	403	rBV	9670	13961	0.16%	0.015%
16	5.787	454	459	462	rBV5	6422	9992	0.11%	0.011%
17	6.734	614	620	624	rBV4	10557	17560	0.20%	0.019%
18	6.899	639	648	656	rVB	444538	711929	7.95%	0.769%
19	7.063	669	676	689	rVB	1741350	2712483	30.28%	2.932%
20	7.252	701	708	720	rBV	1636353	2567517	28.66%	2.775%
21	7.346	720	724	729	rVV5	8944	14865	0.17%	0.016%
22	7.422	731	737	739	rBV7	6356	9400	0.10%	0.010%
23	7.716	779	787	794	rBV	1633204	2577381	28.77%	2.786%
24	7.793	796	800	805	rVV	39717	56274	0.63%	0.061%
25	7.969	823	830	831	rBV7	10765	14013	0.16%	0.015%
26	8.328	884	891	902	rVB5	13834	43542	0.49%	0.047%
27	8.440	902	910	919	rBV	1265270	1982115	22.13%	2.142%
28	8.546	919	928	933	rVB2	22078	45123	0.50%	0.049%
29	8.816	968	974	979	rBV	128683	203858	2.28%	0.220%
30	8.881	979	985	992	rVB	1908673	3041102	33.95%	3.287%
31	9.052	1009	1014	1019	rVB2	35163	50388	0.56%	0.054%
32	9.599	1098	1107	1121	rBV	1365500	2188488	24.43%	2.365%
33	9.793	1136	1140	1144	rVB	11866	18744	0.21%	0.020%
34	9.846	1144	1149	1154	rBV6	9864	13789	0.15%	0.015%
35	9.934	1159	1164	1171	rBV6	5505	9380	0.10%	0.010%
36	9.999	1171	1175	1179	rBV2	17134	24543	0.27%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010827.D
 Acq On : 25 Jun 2022 14:29
 Operator : CG/JU
 Sample : N3355-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0D2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	10.140	1191	1199	1208	rBV	2076221	3280379	36.62%	3.546%
38	10.310	1223	1228	1235	rVB9	14635	25031	0.28%	0.027%
39	10.428	1243	1248	1255	rVB9	15694	37467	0.42%	0.040%
40	10.516	1255	1263	1269	rBV	2178351	3604738	40.24%	3.896%
41	10.563	1269	1271	1279	rVB3	38972	59404	0.66%	0.064%
42	10.657	1279	1287	1299	rBV	1962071	3248916	36.27%	3.512%
43	10.887	1319	1326	1330	rBV9	7096	14507	0.16%	0.016%
44	11.075	1353	1358	1363	rBV8	5489	11532	0.13%	0.012%
45	11.169	1363	1374	1382	rVV	63596	113953	1.27%	0.123%
46	11.328	1395	1401	1406	rBV3	26122	46591	0.52%	0.050%
47	11.798	1477	1481	1484	rBV3	9567	15116	0.17%	0.016%
48	11.840	1484	1488	1492	rBV2	21725	31730	0.35%	0.034%
49	11.951	1503	1507	1511	rVB5	10616	15314	0.17%	0.017%
50	12.046	1517	1523	1528	rBV10	4647	11304	0.13%	0.012%
51	12.110	1528	1534	1538	rVV	47879	73870	0.82%	0.080%
52	12.328	1567	1571	1576	rVB8	7281	13205	0.15%	0.014%
53	12.675	1626	1630	1634	rVV7	6383	11695	0.13%	0.013%
54	12.745	1636	1642	1647	rBV8	10386	20043	0.22%	0.022%
55	12.993	1679	1684	1687	rBV4	13966	18608	0.21%	0.020%
56	13.098	1697	1702	1708	rBV8	5472	12492	0.14%	0.014%
57	13.222	1719	1723	1727	rBV6	11391	14536	0.16%	0.016%
58	13.298	1727	1736	1742	rBV	95864	156094	1.74%	0.169%
59	13.622	1785	1791	1795	rBV8	5973	10304	0.12%	0.011%
60	13.704	1799	1805	1810	rBV3	18553	29328	0.33%	0.032%
61	13.798	1814	1821	1829	rBV	3690377	4975358	55.55%	5.378%
62	13.887	1833	1836	1840	rVB5	6781	10088	0.11%	0.011%
63	14.069	1857	1867	1879	rBV	4229310	6228390	69.53%	6.732%
64	14.240	1892	1896	1901	rVB7	6539	11645	0.13%	0.013%
65	14.375	1910	1919	1929	rBV	2969060	4284439	47.83%	4.631%
66	14.469	1930	1935	1940	rVB4	18736	29036	0.32%	0.031%
67	14.592	1947	1956	1972	rBV	252651	414925	4.63%	0.448%
68	14.810	1988	1993	1997	rVB8	15054	21011	0.23%	0.023%
69	15.063	2029	2036	2044	rVV	60903	108422	1.21%	0.117%
70	15.134	2044	2048	2053	rVB3	10881	14848	0.17%	0.016%
71	15.375	2082	2089	2097	rBV	5406130	7495732	83.68%	8.102%
72	15.492	2103	2109	2124	rBV	906367	1260938	14.08%	1.363%
73	15.616	2125	2130	2136	rVB	63809	100781	1.13%	0.109%
74	15.751	2148	2153	2161	rVB3	31714	50021	0.56%	0.054%
75	15.845	2166	2169	2177	rVB9	5366	9512	0.11%	0.010%
76	15.998	2191	2195	2200	rBV8	10021	15359	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010827.D
 Acq On : 25 Jun 2022 14:29
 Operator : CG/JU
 Sample : N3355-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0D2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

77	16.163	2219	2223	2227	rBV5	18584	29489	0.33%	0.032%
78	16.739	2318	2321	2329	rVB4	11638	17120	0.19%	0.019%
79	16.816	2331	2334	2341	rVB7	11039	14750	0.16%	0.016%
80	16.916	2348	2351	2360	rBV4	14281	24779	0.28%	0.027%
81	17.016	2366	2368	2373	rVB6	7301	10219	0.11%	0.011%
82	17.139	2381	2389	2399	rBV	3216844	4280918	47.79%	4.627%
83	17.239	2399	2406	2421	rVV	5465366	7524693	84.01%	8.133%
84	17.392	2430	2432	2437	rVB6	6952	9873	0.11%	0.011%
85	17.445	2439	2441	2447	rVB	12367	14687	0.16%	0.016%
86	17.522	2451	2454	2462	rBV8	7720	14144	0.16%	0.015%
87	17.828	2500	2506	2515	rBV	433346	553090	6.17%	0.598%
88	17.992	2531	2534	2537	rBV5	9996	11784	0.13%	0.013%
89	18.292	2582	2585	2589	rBV6	17292	19610	0.22%	0.021%
90	18.610	2635	2639	2643	rBV	62066	69886	0.78%	0.076%
91	19.063	2712	2716	2722	rVB2	68388	93800	1.05%	0.101%
92	19.133	2724	2728	2733	rVV	61591	82216	0.92%	0.089%
93	19.486	2783	2788	2796	rBV	6115248	8058838	89.97%	8.710%
94	21.251	3083	3088	3093	rBV	3717460	4489317	50.12%	4.852%
95	23.468	3458	3465	3474	rVB2	4793643	8957301	100.00%	9.681%
96	23.621	3485	3491	3504	rVB	2479611	4842761	54.06%	5.234%




Sum of corrected areas: 92520892

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010827.D
Acq On : 25 Jun 2022 14:29
Operator : CG/JU
Sample : N3355-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0D2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

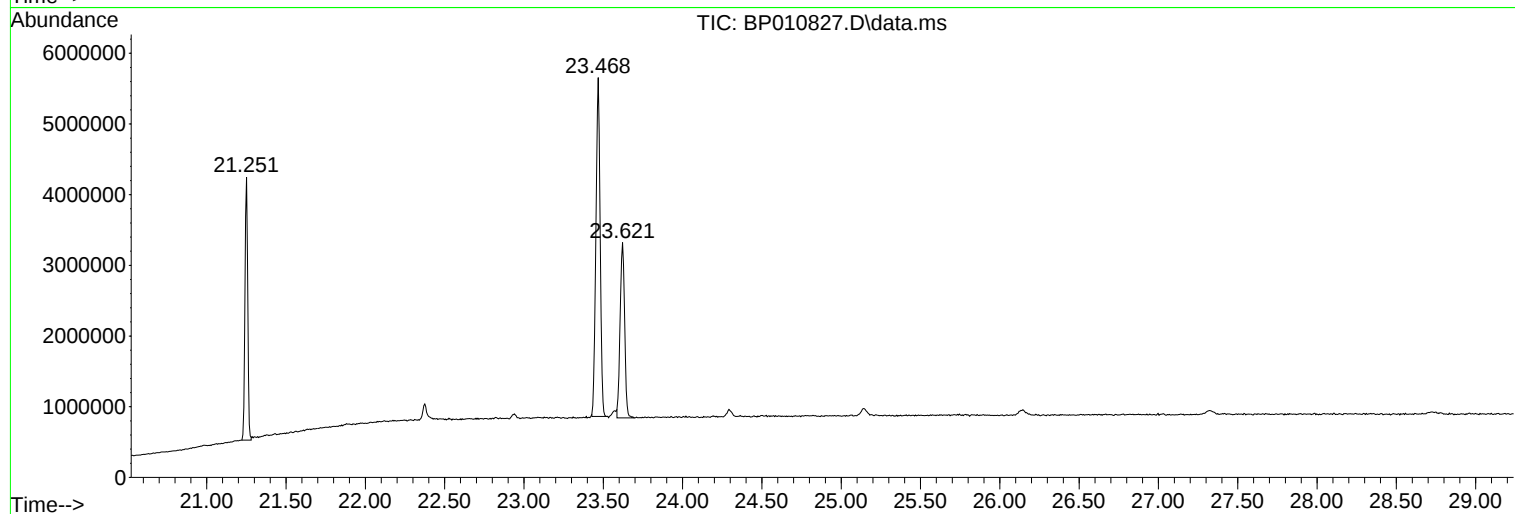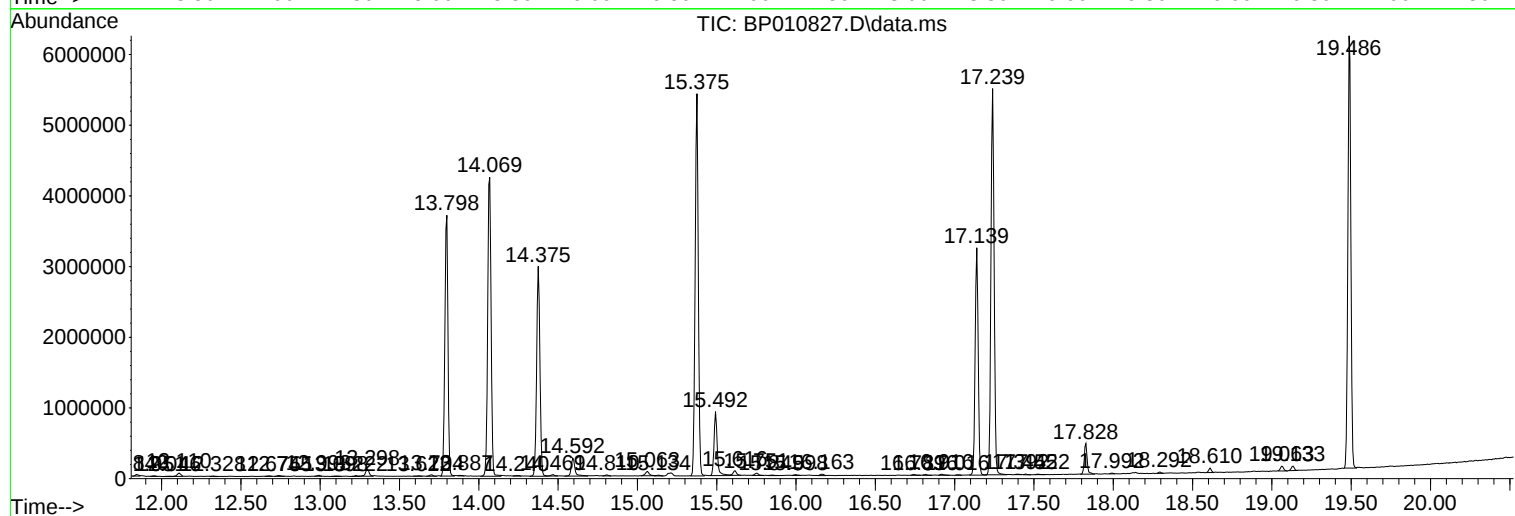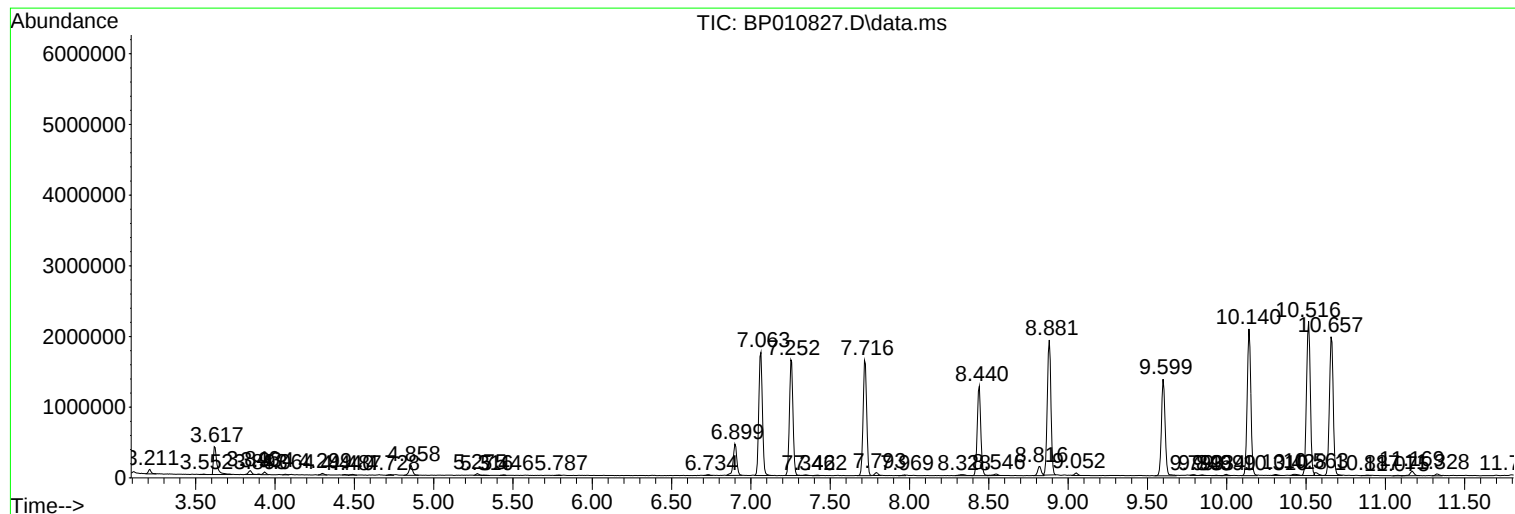

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010827.D
Acq On : 25 Jun 2022 14:29
Operator : CG/JU
Sample : N3355-16
Misc :
ALS Vial : 8 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
EY0D2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
17.828	2.58 ng/ul	553090	Phenanthrene-d10	17.139	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	99
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	90
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	89
4	Ethanone, 1-(5,6,7,8-tetrahydro-...	220	C14H20O2	071596-88-8	87
5	1,3-Pentadiene, 1,1-diphenyl-, (Z)-	220	C17H16	015295-31-5	50

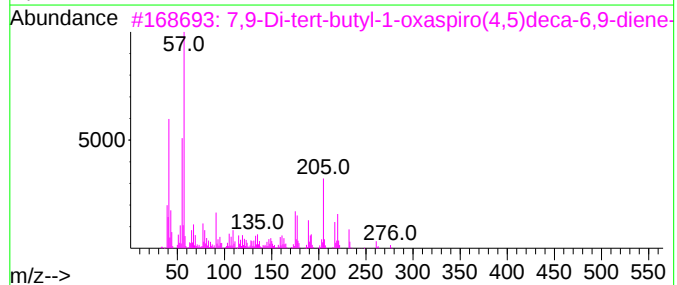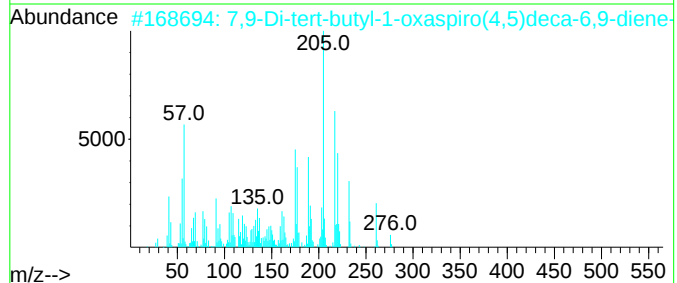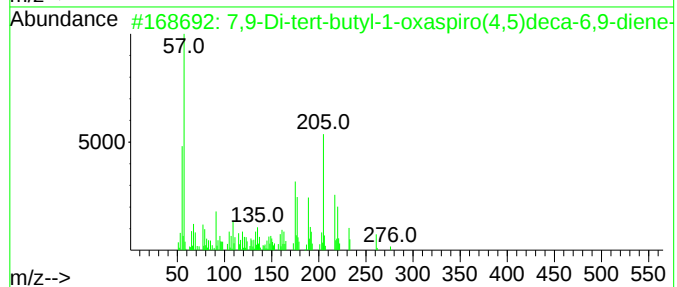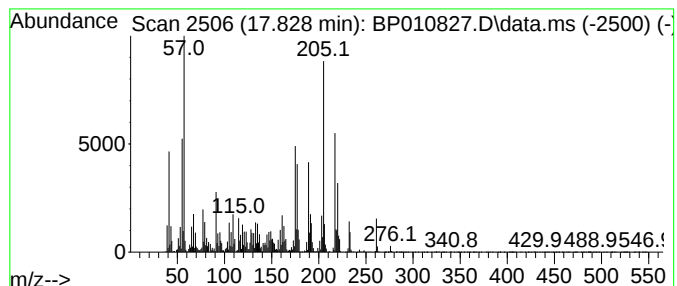

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010827.D
Acq On : 25 Jun 2022 14:29
Operator : CG/JU
Sample : N3355-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0D2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	17.828	2.6	ng/u1	553090	4	17.139	4280920	20.0