

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010832.D
 Acq On : 25 Jun 2022 17:18
 Operator : CG/JU
 Sample : N3355-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	17	21	24	rBV	63385	70636	0.76%	0.076%
2	3.487	65	68	75	rVB	12031	19395	0.21%	0.021%
3	3.616	87	90	115	rVB	684588	963017	10.31%	1.041%
4	3.840	123	128	133	rBV	58071	85654	0.92%	0.093%
5	3.893	135	137	140	rVV4	9833	12390	0.13%	0.013%
6	3.934	140	144	150	rVB2	39440	54929	0.59%	0.059%
7	4.452	227	232	235	rBV3	29129	41889	0.45%	0.045%
8	4.487	235	238	243	rVB2	10738	16510	0.18%	0.018%
9	4.722	274	278	283	rBV2	9882	14856	0.16%	0.016%
10	4.858	292	301	310	rBV2	169860	270139	2.89%	0.292%
11	5.440	396	400	407	rBV	12569	18394	0.20%	0.020%
12	6.899	637	648	660	rVB	534606	807589	8.65%	0.873%
13	7.057	668	675	683	rBV	1713715	2648417	28.36%	2.863%
14	7.134	684	688	695	rVB	21643	35355	0.38%	0.038%
15	7.252	701	708	717	rBV	1728522	2639626	28.26%	2.854%
16	7.346	720	724	730	rVB4	10170	16819	0.18%	0.018%
17	7.716	780	787	795	rBV	1847913	2838441	30.39%	3.069%
18	7.793	795	800	804	rVB3	12086	17384	0.19%	0.019%
19	8.434	902	909	918	rBV	1404325	2187724	23.42%	2.365%
20	8.881	977	985	997	rBV	1866676	2992094	32.04%	3.235%
21	9.310	1053	1058	1062	rBV4	10518	17252	0.18%	0.019%
22	9.598	1100	1107	1115	rBV	1331728	2101163	22.50%	2.272%
23	10.140	1190	1199	1210	rBV	2017943	3277893	35.10%	3.544%
24	10.516	1255	1263	1271	rBV	2338986	3925582	42.03%	4.244%
25	10.657	1279	1287	1298	rBV	2034021	3326536	35.62%	3.596%
26	11.881	1490	1495	1499	rVB8	6090	11119	0.12%	0.012%
27	12.110	1527	1534	1541	rVB	43787	72152	0.77%	0.078%
28	13.098	1695	1702	1707	rBV8	6594	12161	0.13%	0.013%
29	13.210	1716	1721	1727	rVB5	13331	25747	0.28%	0.028%
30	13.792	1812	1820	1829	rBV	3678444	4919381	52.67%	5.318%
31	14.063	1858	1866	1878	rBV	4065115	5972256	63.95%	6.457%
32	14.375	1911	1919	1930	rBV	3036340	4426166	47.39%	4.785%
33	14.592	1950	1956	1967	rBV	307609	462176	4.95%	0.500%
34	14.734	1977	1980	1984	rBV5	6500	9987	0.11%	0.011%
35	14.804	1988	1992	1999	rVB9	13829	24115	0.26%	0.026%
36	15.198	2054	2059	2065	rBV3	13478	24961	0.27%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010832.D
 Acq On : 25 Jun 2022 17:18
 Operator : CG/JU
 Sample : N3355-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	15.375	2082	2089	2103	rBV	5227088	7300059	78.16%	7.892%
38	15.492	2103	2109	2124	rBV	913218	1283324	13.74%	1.387%
39	15.616	2125	2130	2135	rVB	59331	89004	0.95%	0.096%
40	16.163	2219	2223	2231	rVB5	21738	35496	0.38%	0.038%
41	16.816	2330	2334	2340	rVB8	10429	16879	0.18%	0.018%
42	16.922	2348	2352	2355	rBV5	11841	16198	0.17%	0.018%
43	17.139	2382	2389	2396	rVV	3244057	4424225	47.37%	4.783%
44	17.239	2399	2406	2418	rBV	5181042	7428829	79.54%	8.031%
45	17.833	2504	2507	2512	rVB	32079	36490	0.39%	0.039%
46	19.063	2712	2716	2722	rBV2	64970	90175	0.97%	0.097%
47	19.127	2724	2727	2734	rVB	58490	84979	0.91%	0.092%
48	19.486	2782	2788	2796	rBV	6377202	8045367	86.14%	8.698%
49	20.980	3039	3042	3046	rBV2	105619	129735	1.39%	0.140%
50	21.251	3083	3088	3093	rBV	3607152	4645459	49.74%	5.022%
51	23.468	3458	3465	3475	rVB2	4885537	9339568	100.00%	10.097%
52	23.621	3484	3491	3501	rVB2	2592380	5171889	55.38%	5.591%




Sum of corrected areas: 92497581

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010832.D
Acq On : 25 Jun 2022 17:18
Operator : CG/JU
Sample : N3355-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

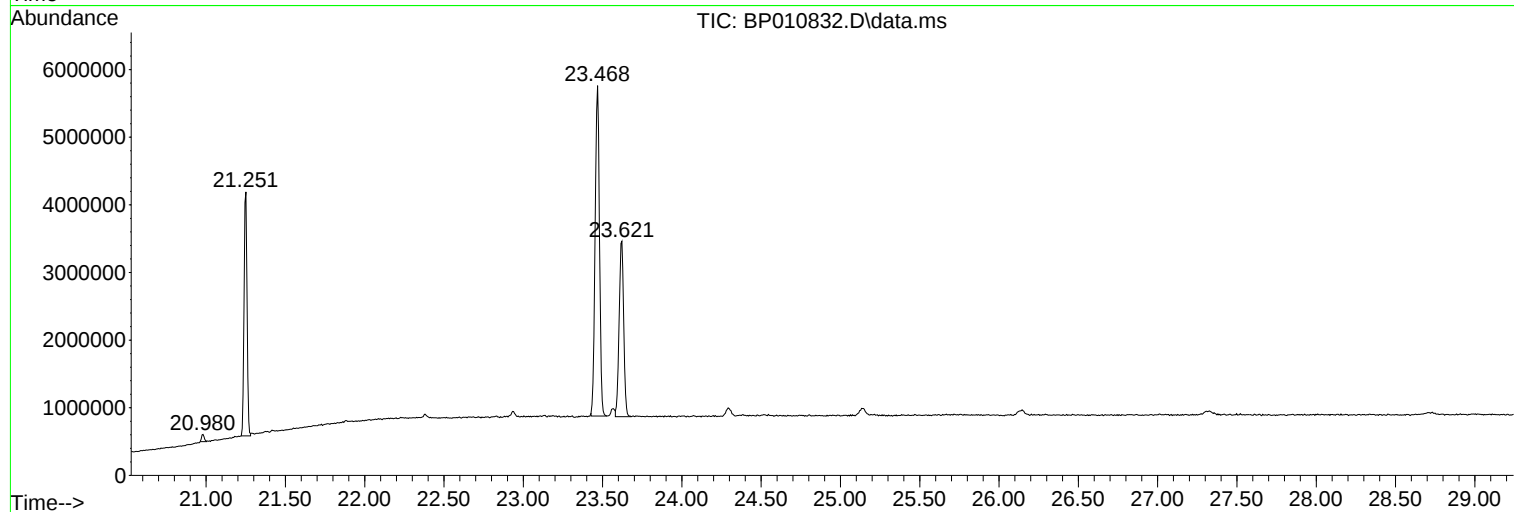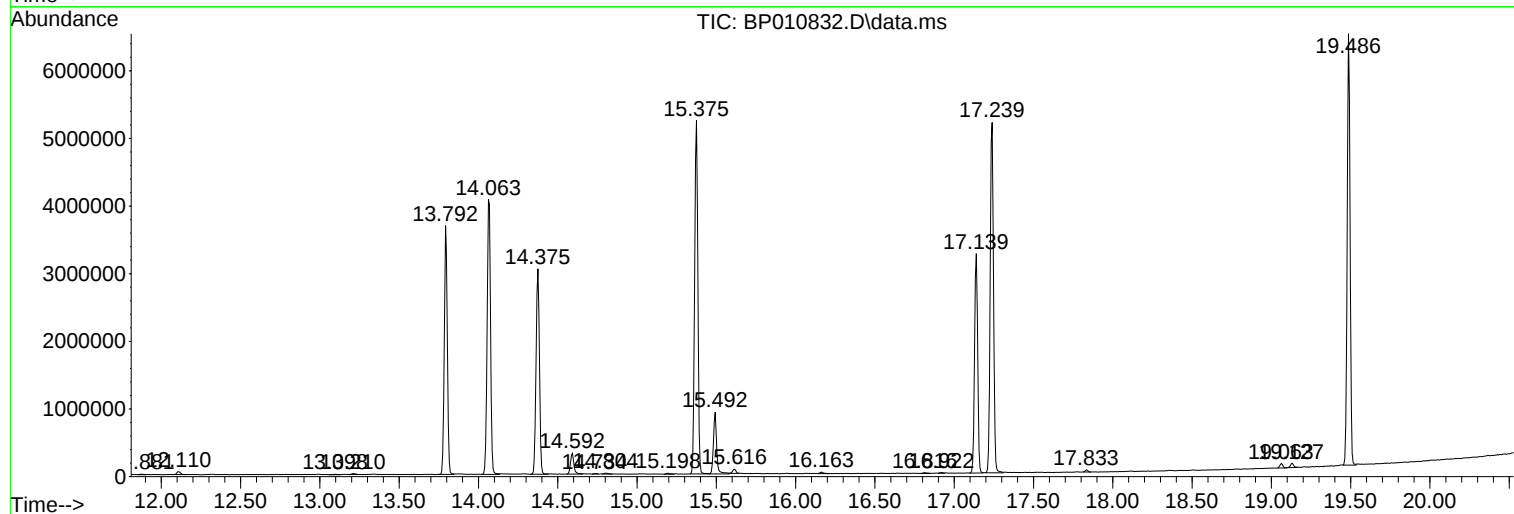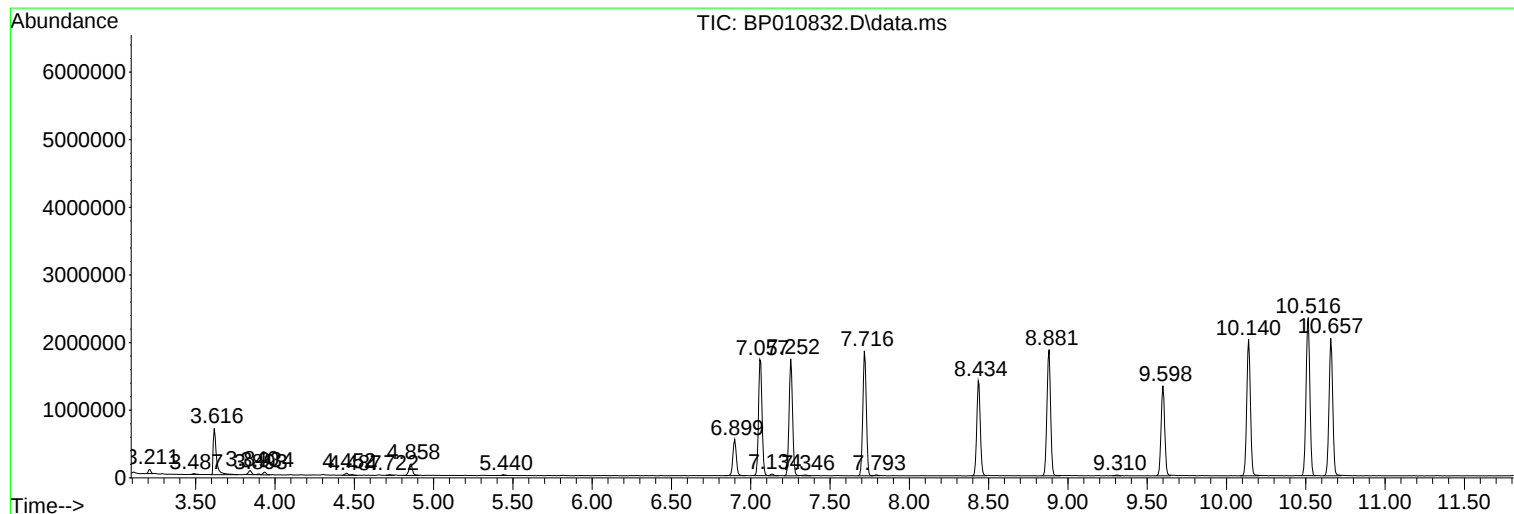

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010832.D
Acq On : 25 Jun 2022 17:18
Operator : CG/JU
Sample : N3355-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010832.D
Acq On : 25 Jun 2022 17:18
Operator : CG/JU
Sample : N3355-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc