

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010833.D
 Acq On : 25 Jun 2022 17:51
 Operator : CG/JU
 Sample : N3355-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0C7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	13	15	18	rBV3	10466	11805	0.14%	0.015%
2	3.211	18	21	29	rVB	52757	67909	0.79%	0.085%
3	3.617	87	90	108	rBV	439760	651004	7.57%	0.817%
4	3.840	122	128	133	rBV	50948	79723	0.93%	0.100%
5	3.934	140	144	151	rVB	36572	50765	0.59%	0.064%
6	4.305	203	207	212	rBV7	7690	9661	0.11%	0.012%
7	4.481	234	237	244	rBV4	9404	15088	0.18%	0.019%
8	4.652	262	266	272	rVB4	7442	9448	0.11%	0.012%
9	4.723	274	278	282	rVV5	9074	14635	0.17%	0.018%
10	4.858	294	301	309	rVV2	109571	177479	2.06%	0.223%
11	5.440	396	400	406	rVB	9718	16093	0.19%	0.020%
12	6.899	641	648	658	rVB	381840	585588	6.81%	0.735%
13	7.058	665	675	685	rBV	1426676	2172247	25.25%	2.727%
14	7.134	685	688	694	rVB	11929	19464	0.23%	0.024%
15	7.252	700	708	716	rBV	1395078	2147481	24.97%	2.696%
16	7.340	720	723	728	rVB6	7950	12408	0.14%	0.016%
17	7.717	778	787	794	rBV	1450582	2226966	25.89%	2.796%
18	7.787	794	799	804	rVB7	8189	13186	0.15%	0.017%
19	8.434	903	909	920	rBV	1103733	1687346	19.62%	2.118%
20	8.881	974	985	993	rBV	1497804	2455812	28.55%	3.083%
21	9.305	1052	1057	1063	rVB8	6740	11671	0.14%	0.015%
22	9.599	1098	1107	1118	rBV	1066393	1732642	20.14%	2.175%
23	10.140	1190	1199	1208	rBV	1681092	2716431	31.58%	3.410%
24	10.516	1254	1263	1273	rBV	1814683	3093488	35.96%	3.883%
25	10.658	1279	1287	1297	rBV	1607249	2630695	30.58%	3.302%
26	11.328	1397	1401	1406	rVB8	5423	8739	0.10%	0.011%
27	11.822	1476	1485	1487	rBV9	4649	11212	0.13%	0.014%
28	11.881	1490	1495	1499	rVB7	8127	14189	0.16%	0.018%
29	12.110	1528	1534	1541	rVB	35363	58785	0.68%	0.074%
30	13.210	1717	1721	1724	rBV4	10094	14594	0.17%	0.018%
31	13.340	1737	1743	1747	rVB9	5329	10147	0.12%	0.013%
32	13.793	1814	1820	1829	rBV	2970900	4109381	47.77%	5.159%
33	14.063	1859	1866	1888	rBV	3550112	5068951	58.93%	6.363%
34	14.375	1911	1919	1927	rBV	2430465	3547323	41.24%	4.453%
35	14.587	1950	1955	1964	rBV	248415	385061	4.48%	0.483%
36	14.681	1968	1971	1975	rVV6	5444	8897	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
 Data File : BP010833.D
 Acq On : 25 Jun 2022 17:51
 Operator : CG/JU
 Sample : N3355-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0C7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
 Title : SVOA CALIBRATION

37	14.740	1978	1981	1984	rVV5	5977	8973	0.10%	0.011%
38	14.810	1986	1993	1997	rVB10	11684	20274	0.24%	0.025%
39	15.375	2082	2089	2095	rBV	4508891	6354258	73.87%	7.977%
40	15.416	2095	2096	2103	rVV6	32052	37844	0.44%	0.048%
41	15.493	2103	2109	2124	rVV	793782	1120722	13.03%	1.407%
42	15.616	2124	2130	2134	rVV	49959	74544	0.87%	0.094%
43	16.163	2219	2223	2233	rVB6	18540	32917	0.38%	0.041%
44	16.816	2332	2334	2341	rVB8	11251	13678	0.16%	0.017%
45	17.134	2382	2388	2397	rBV	2649179	3833791	44.57%	4.813%
46	17.240	2399	2406	2419	rVV	4829752	6694314	77.83%	8.403%
47	17.398	2427	2433	2438	rBV10	11122	22710	0.26%	0.029%
48	17.828	2503	2506	2510	rVB6	10694	15006	0.17%	0.019%
49	19.063	2712	2716	2722	rBV	63642	81940	0.95%	0.103%
50	19.128	2723	2727	2731	rBV	59284	87249	1.01%	0.110%
51	19.486	2782	2788	2796	rBV	6150276	7718677	89.73%	9.689%
52	20.975	3039	3041	3048	rVB5	127754	156009	1.81%	0.196%
53	21.251	3083	3088	3093	rBV	3403632	4333007	50.37%	5.439%
54	23.463	3457	3464	3477	rVB2	4491832	8601645	100.00%	10.798%
55	23.616	3484	3490	3500	rVB2	2311061	4607602	53.57%	5.784%




Sum of corrected areas: 79661474

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010833.D
Acq On : 25 Jun 2022 17:51
Operator : CG/JU
Sample : N3355-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

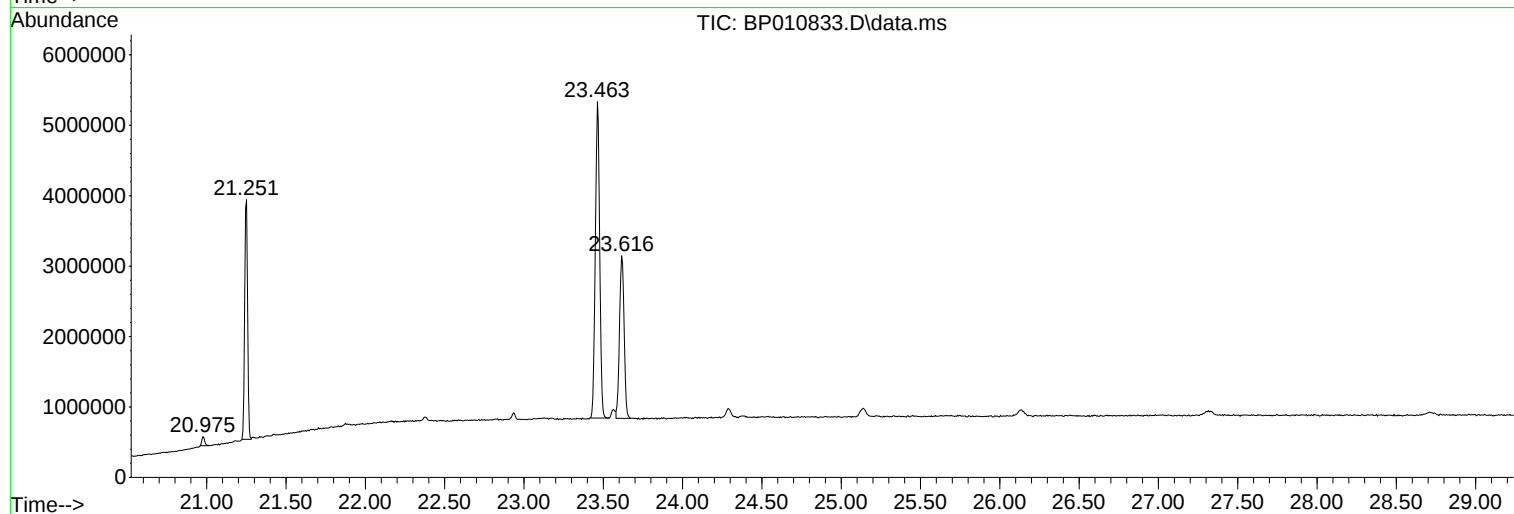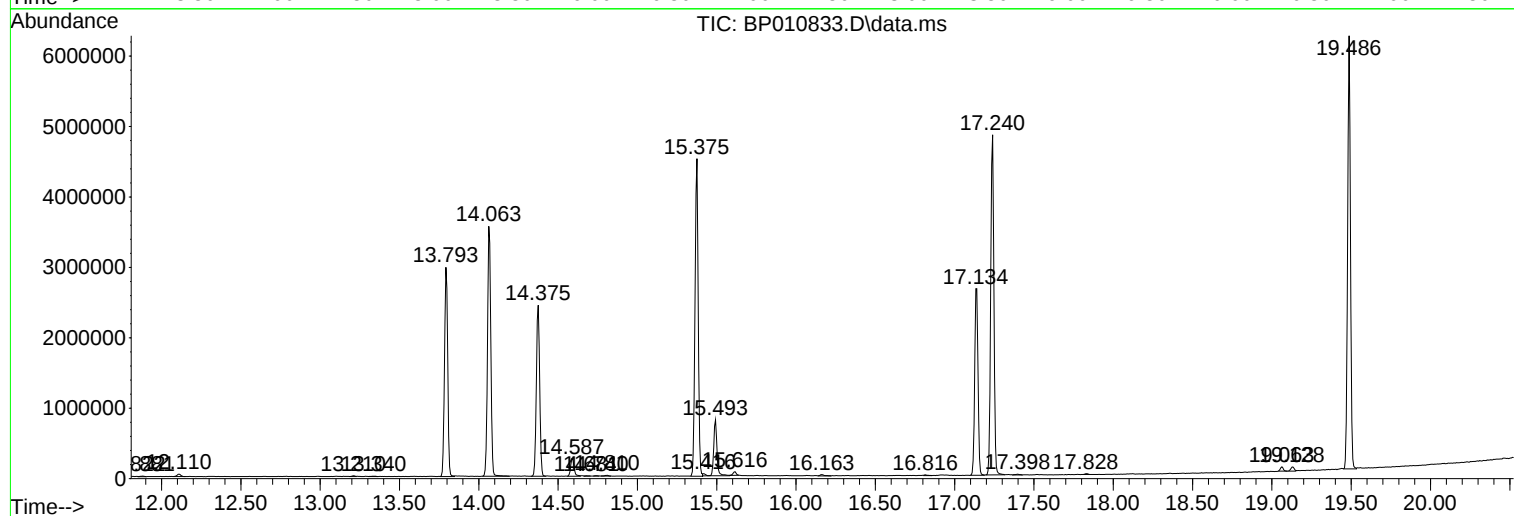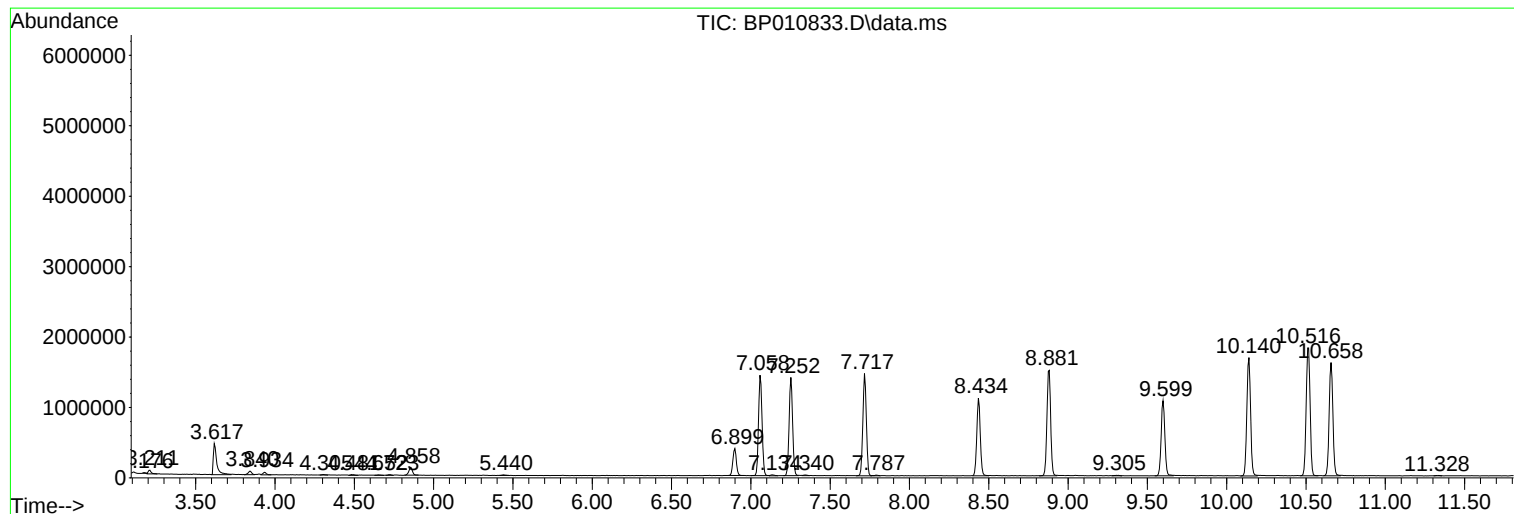

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010833.D
Acq On : 25 Jun 2022 17:51
Operator : CG/JU
Sample : N3355-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062522\
Data File : BP010833.D
Acq On : 25 Jun 2022 17:51
Operator : CG/JU
Sample : N3355-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0C7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
